

Fig. 1a

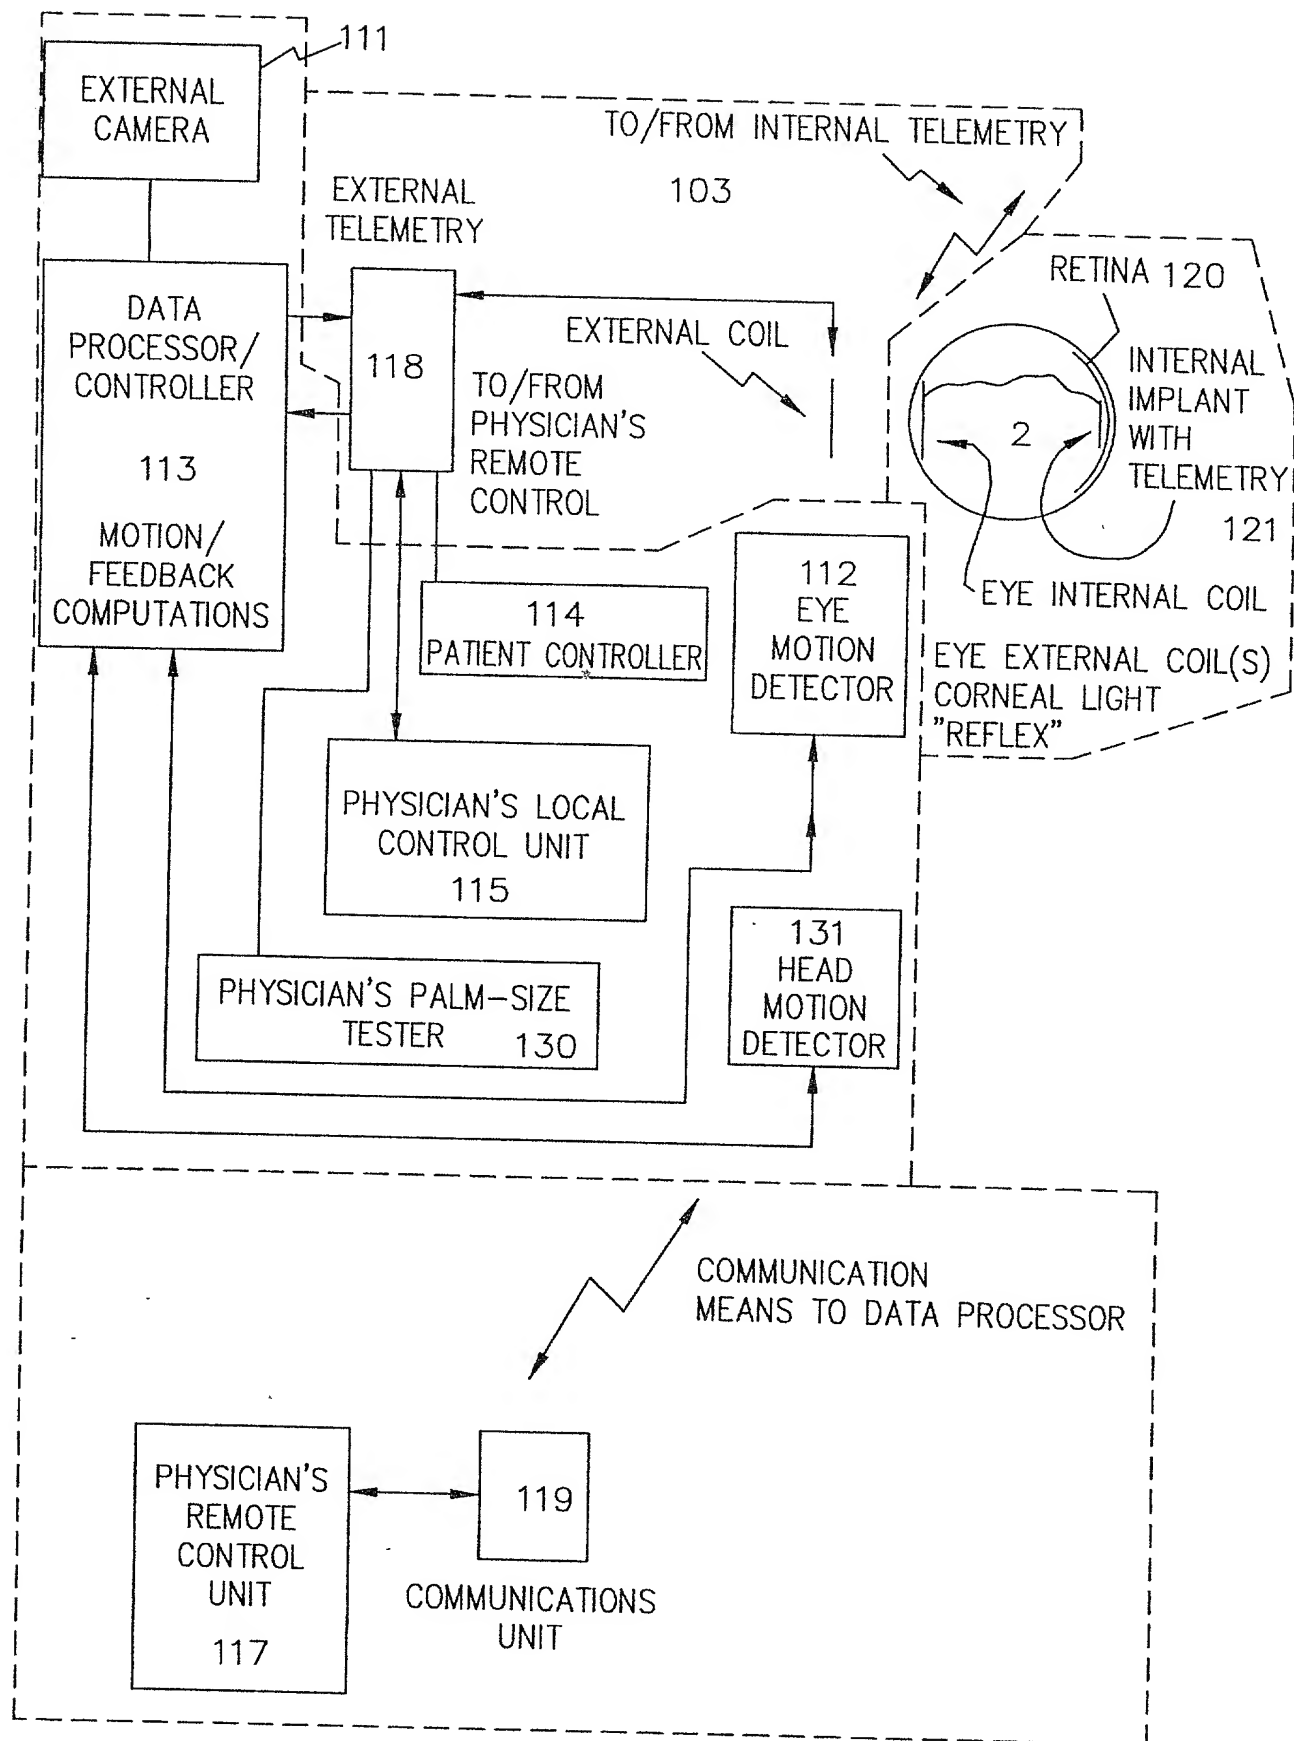


FIGURE 1b

10033576-140901

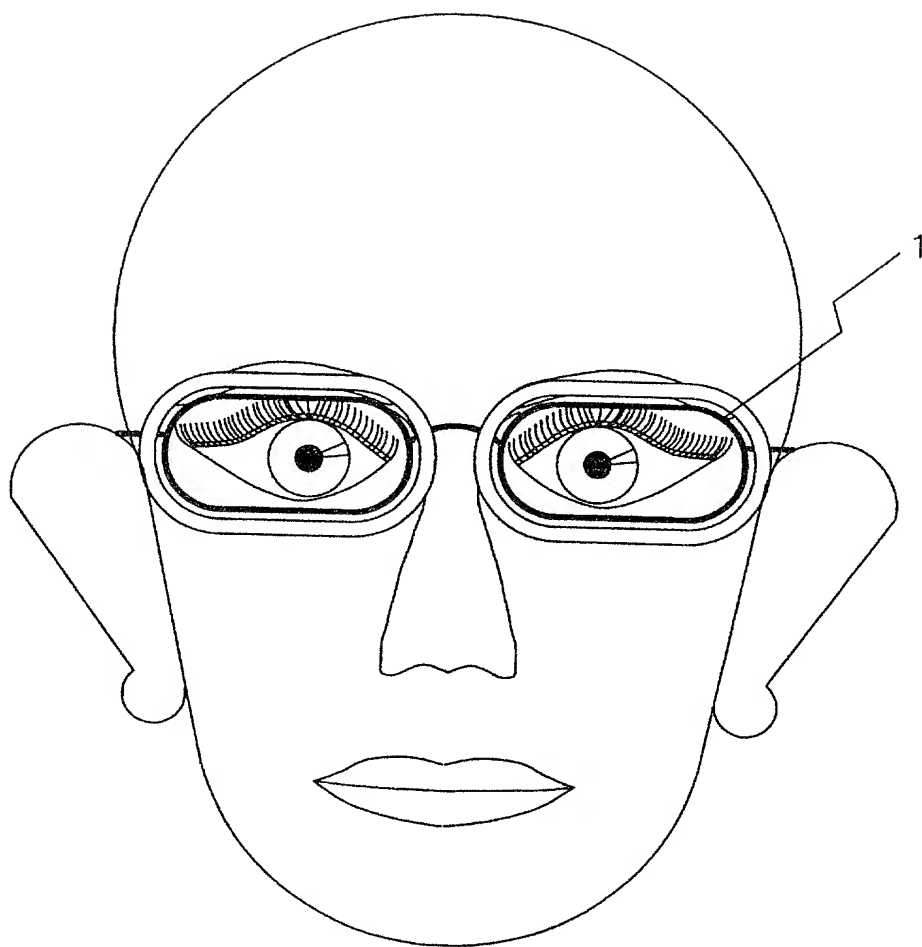


Fig. 1c

10033576, 110901

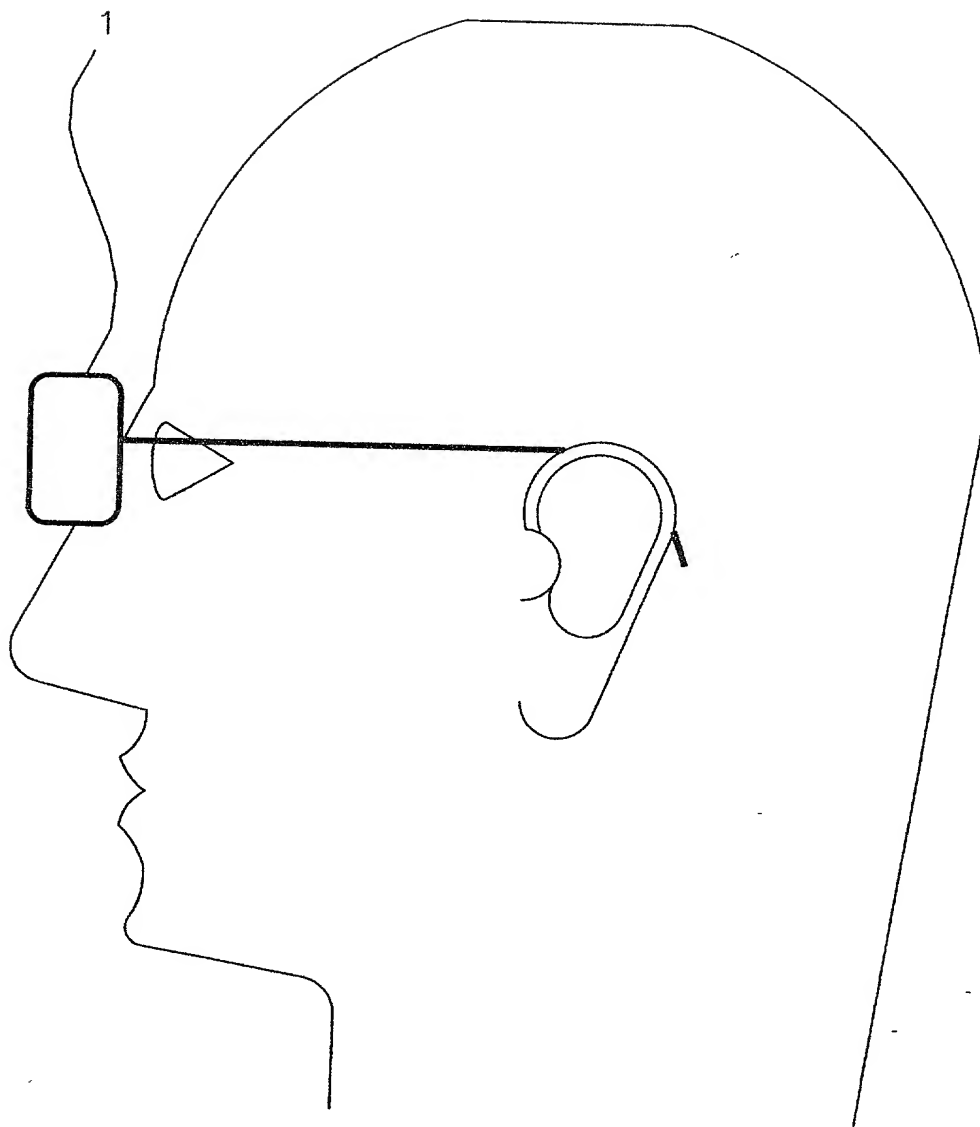


Fig 1d

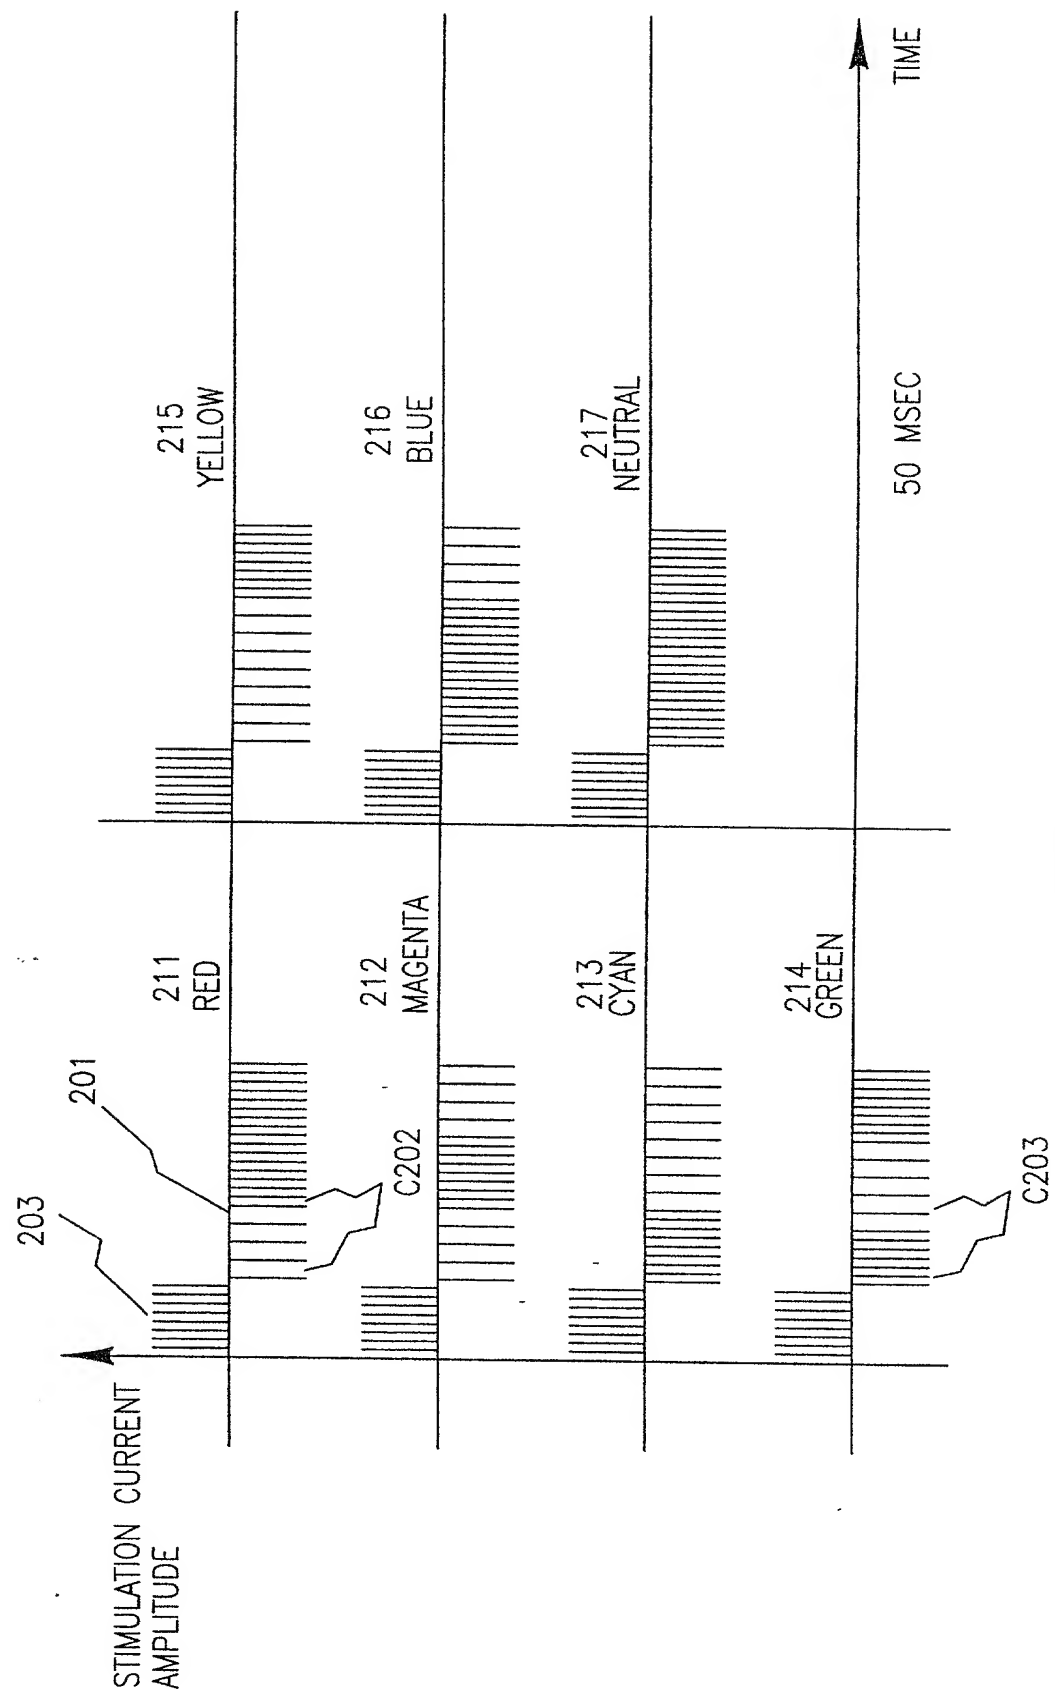


FIGURE 2a  
COLOR CODING

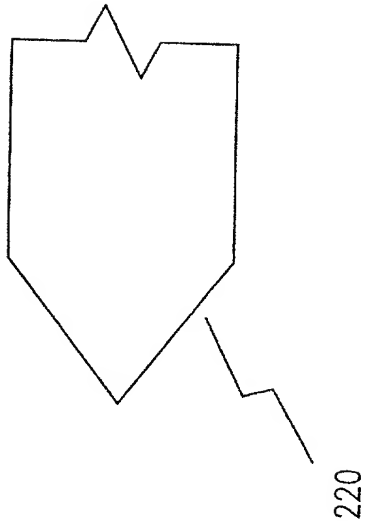
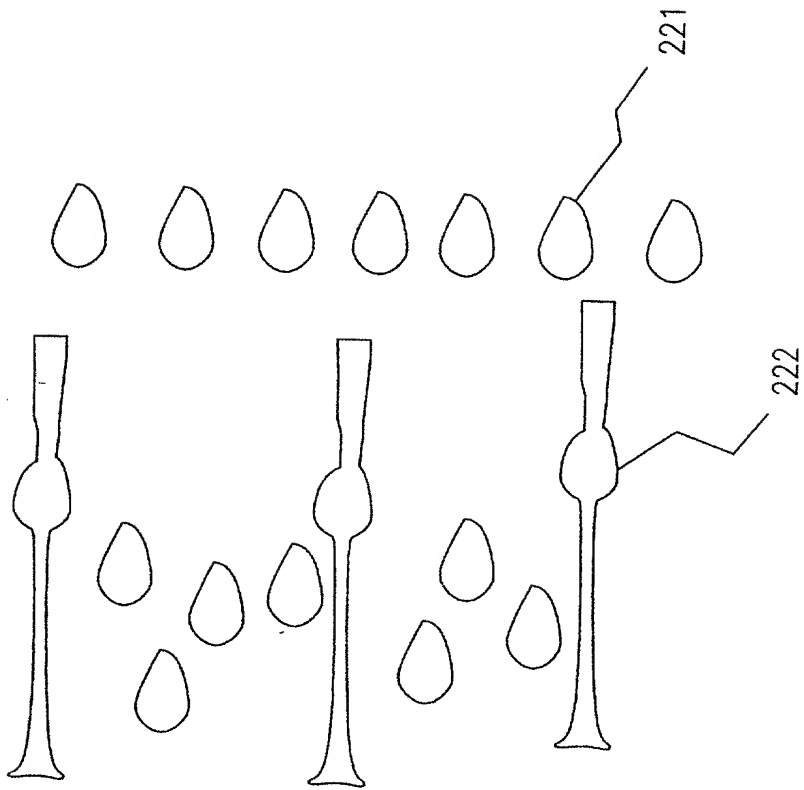


FIGURE 2b


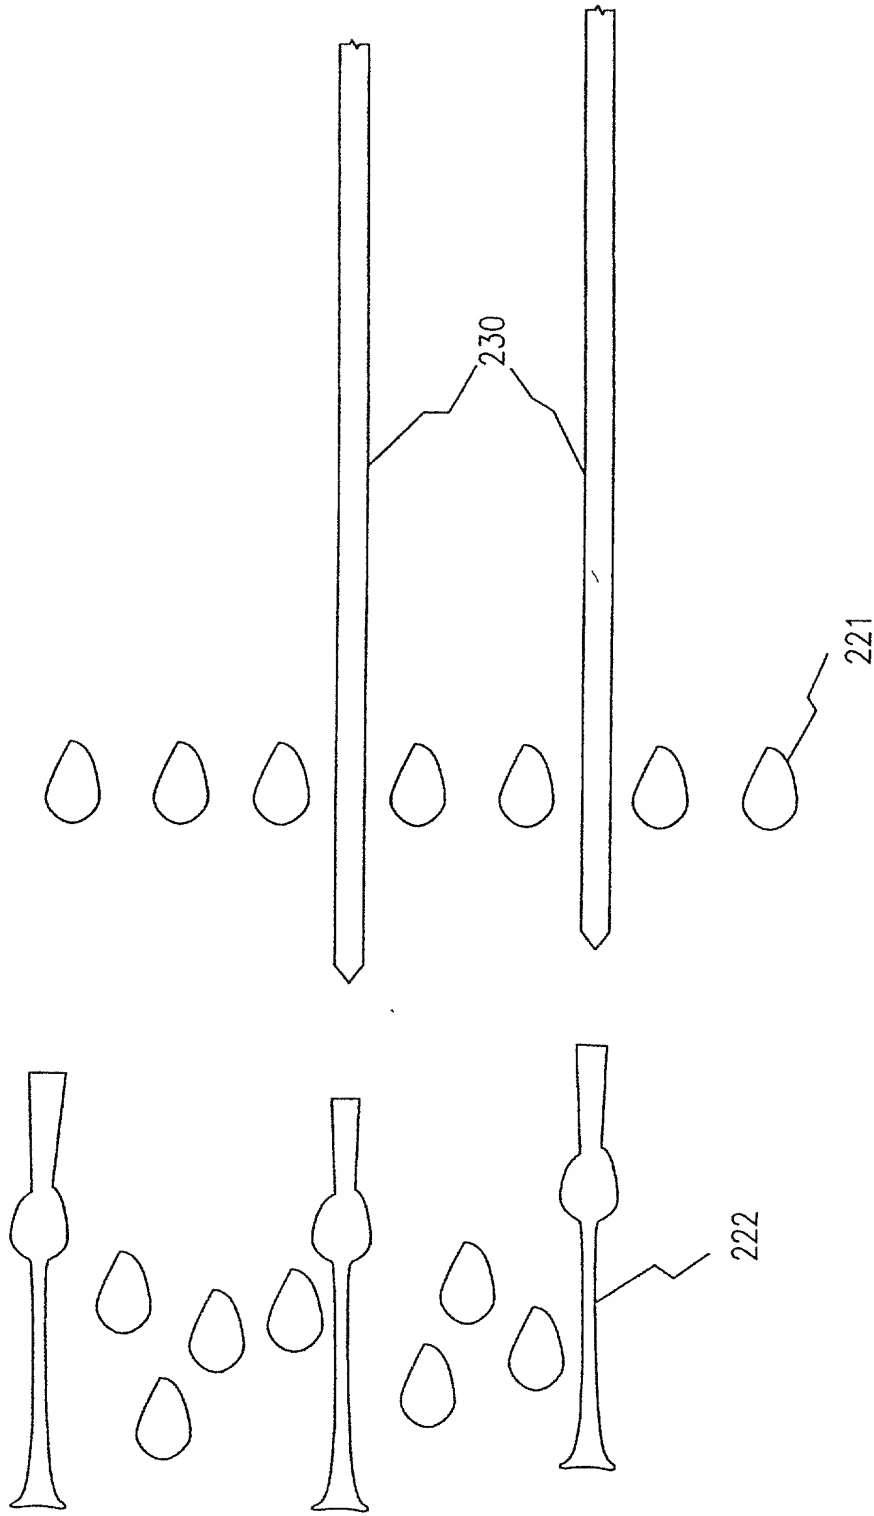


FIGURE 2c

10033576-10901

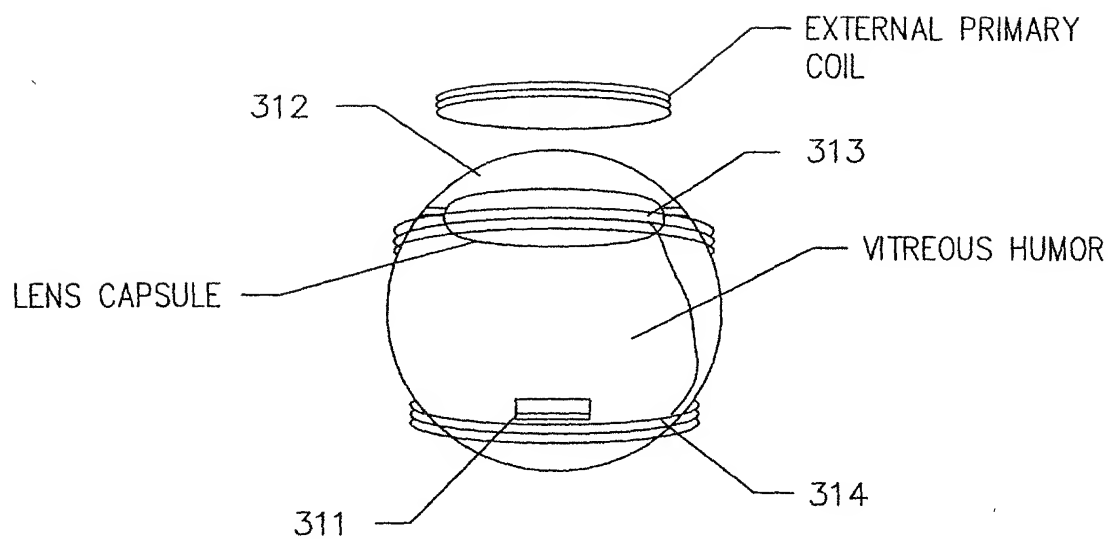

EXTERNAL/INTERNAL TELEMETRY UNIT -  
EXTERNAL COIL/INTERNAL COIL /INTERNAL CHIP

FIGURE 3a



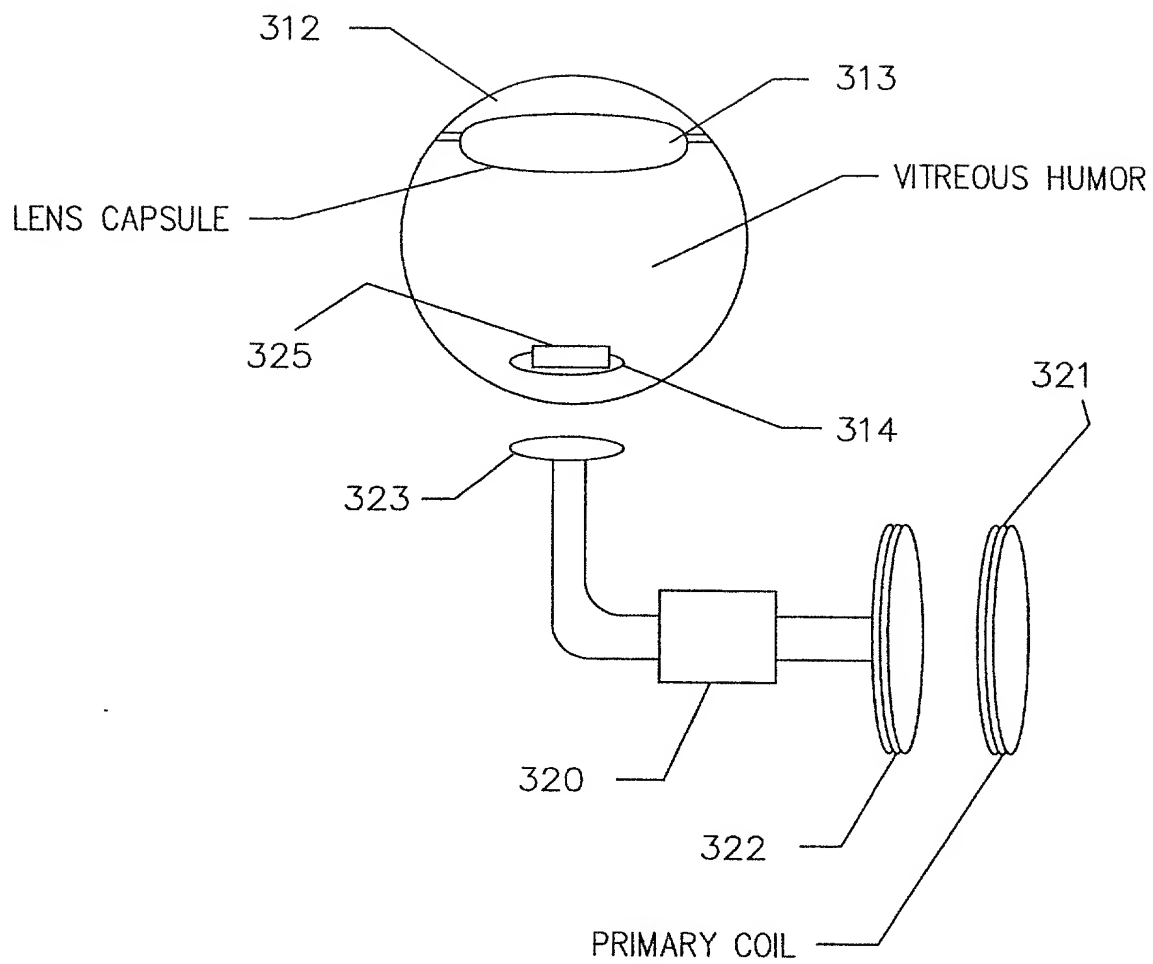


FIGURE 3b

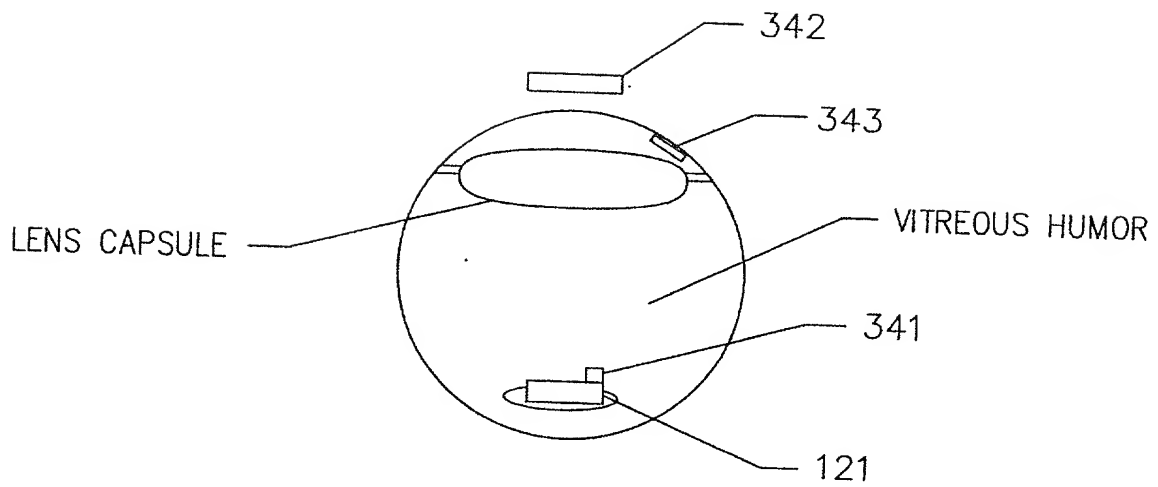


FIGURE 3c




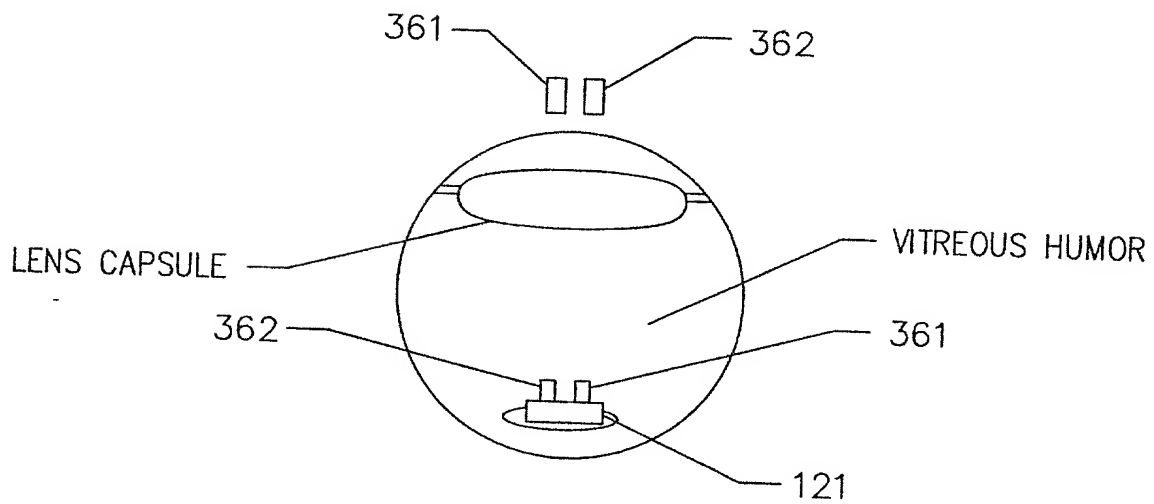


FIGURE 3d

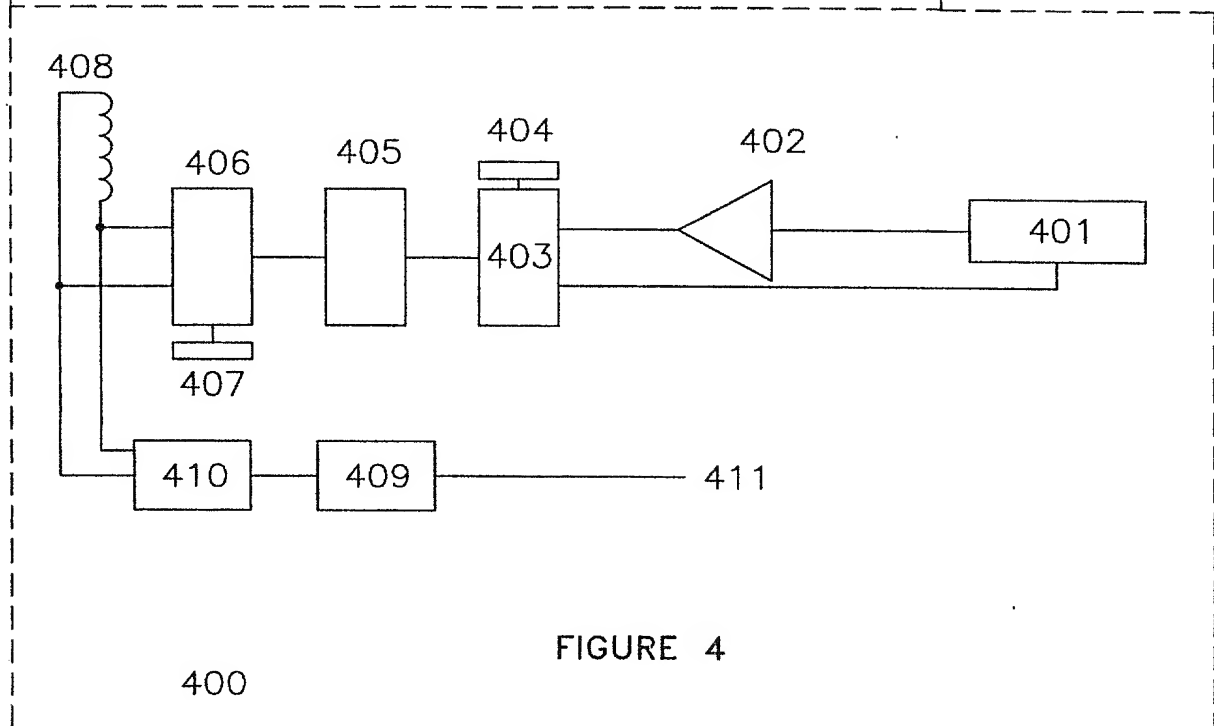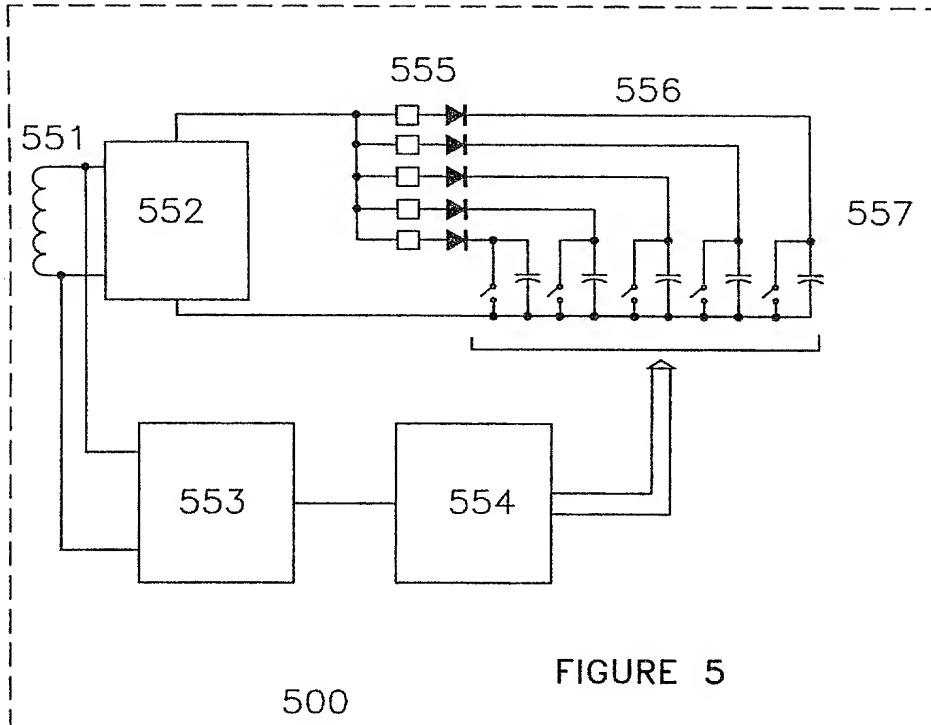

40033576, 40033576

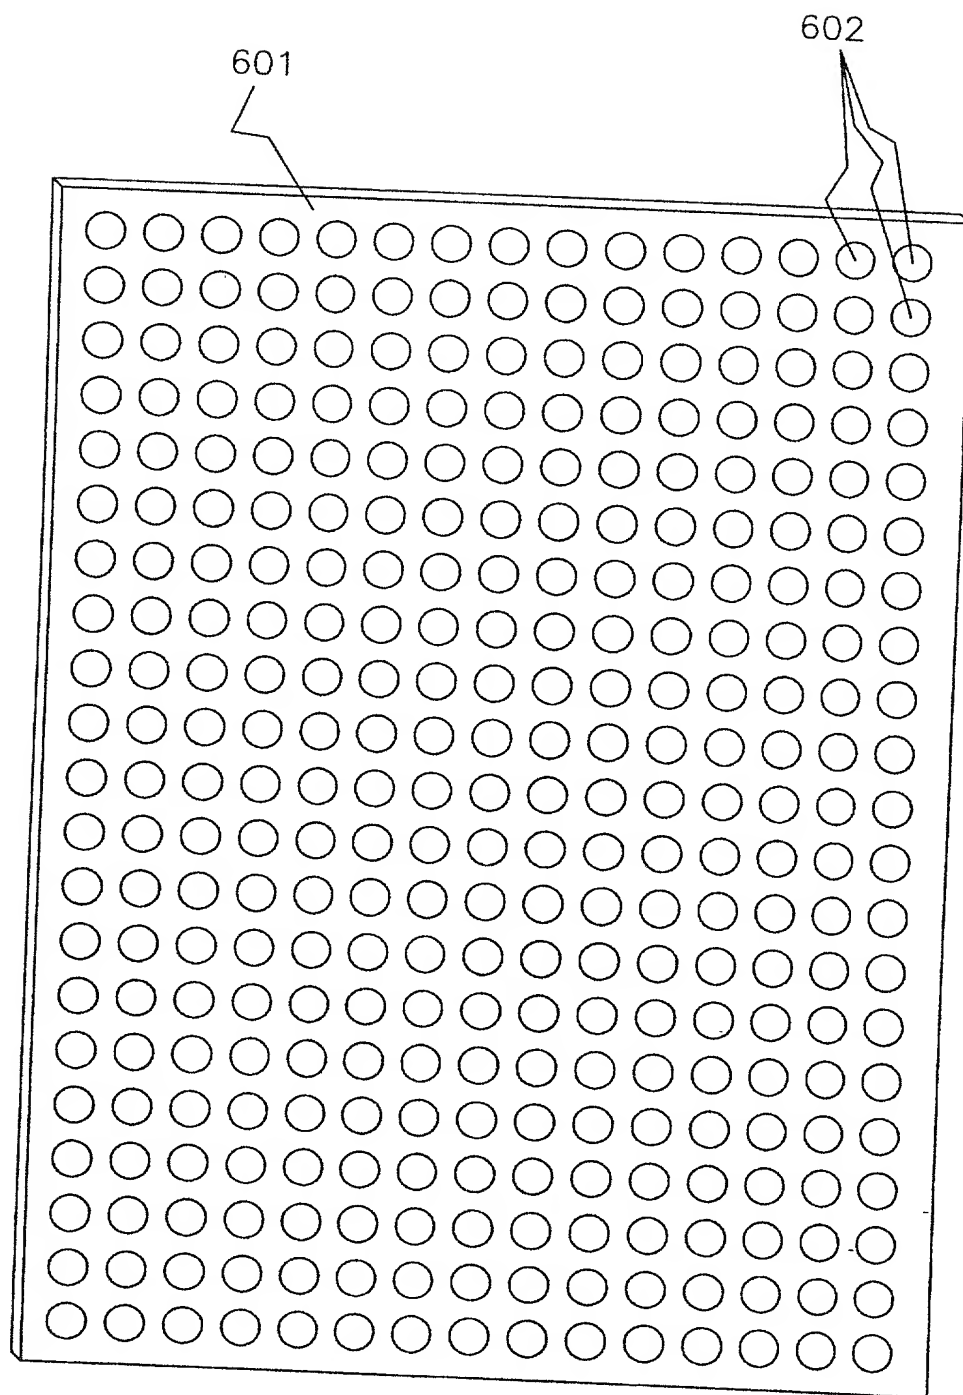

ELECTRODES ON SUBSTRATE  
FIGURE 6a

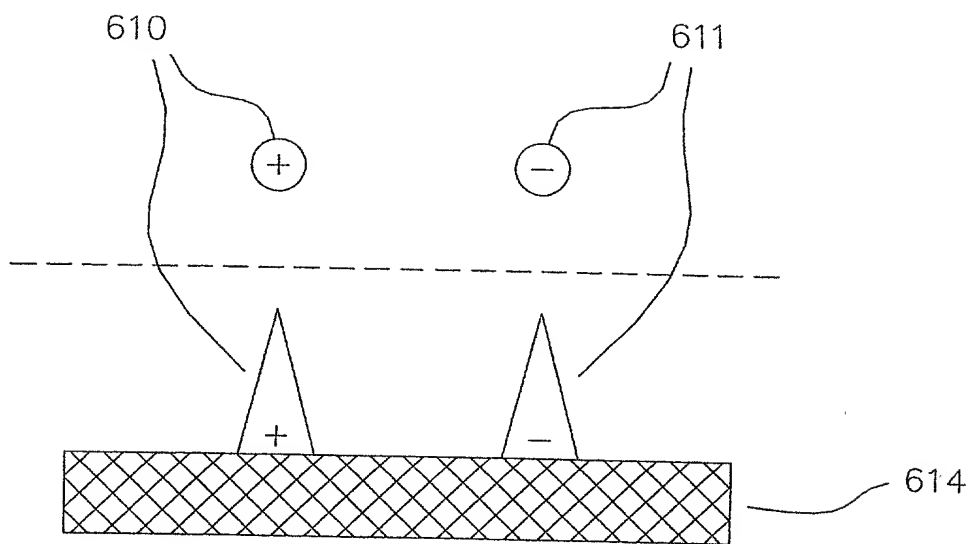


FIGURE 6b


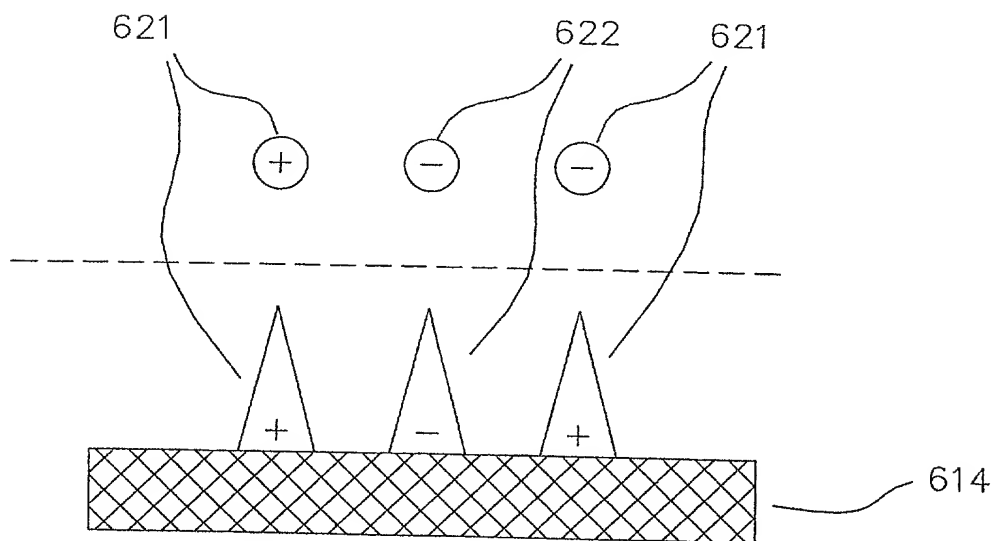




FIGURE 6c

100336-10001

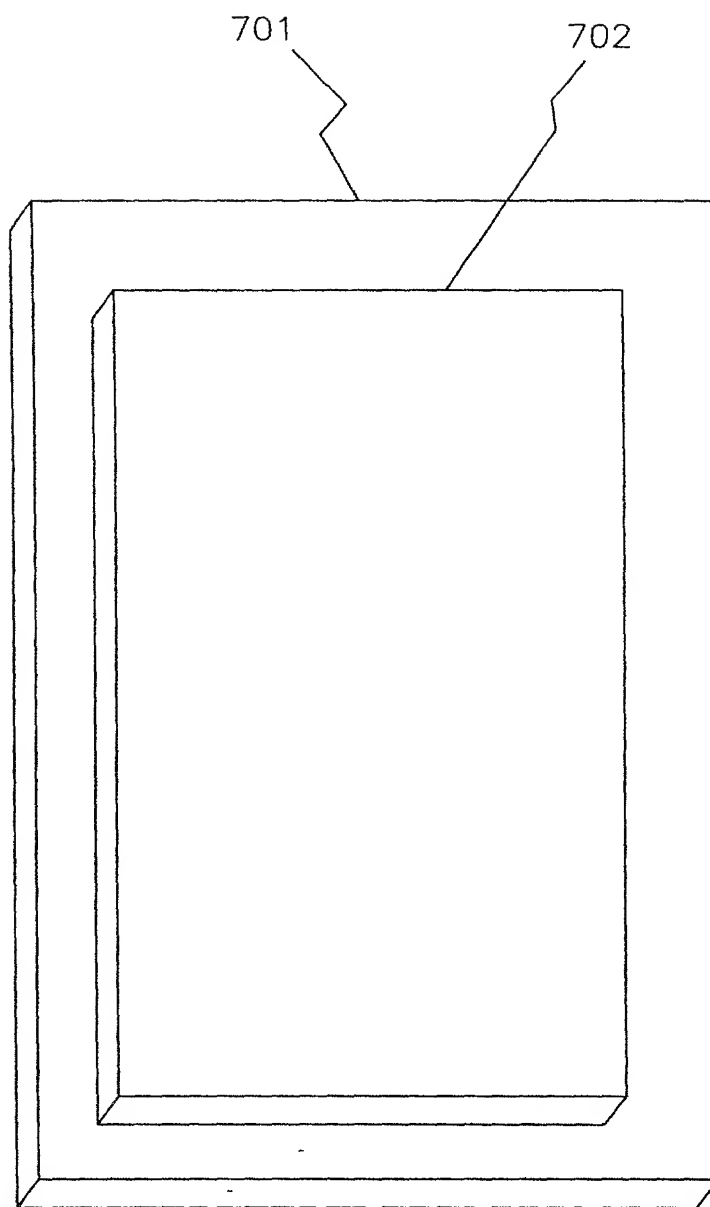


INDIFFERENT ELECTRODE OF MONOPOLAR ELECTRODES

FIGURE 7

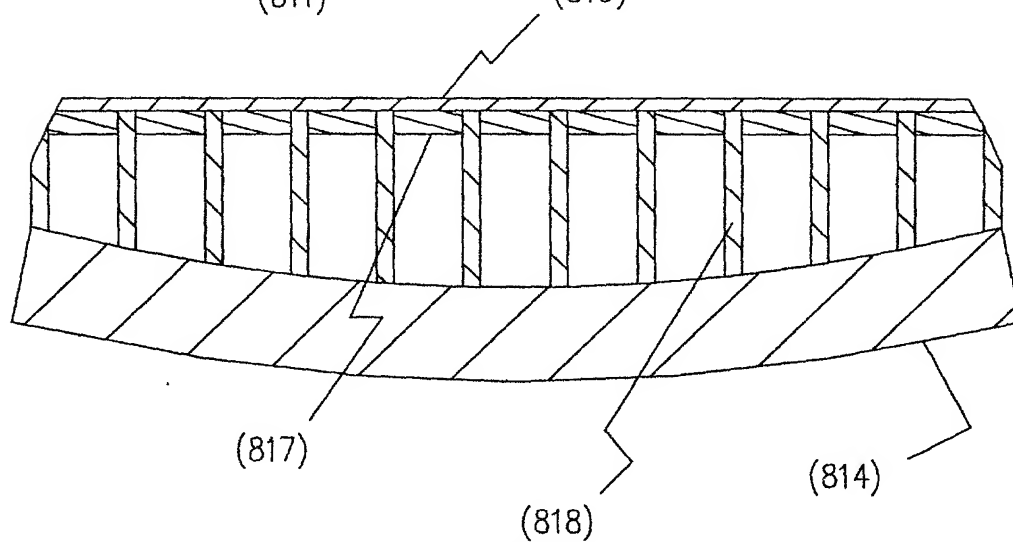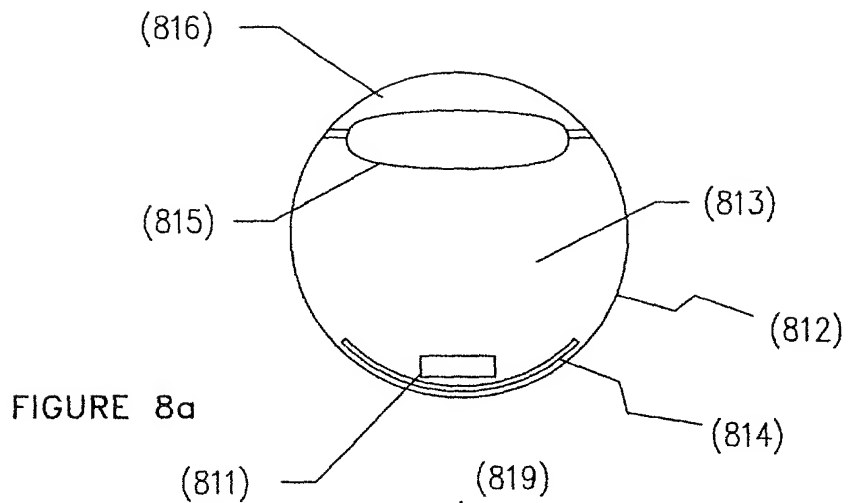

EPIRETINAL ELECTRODES - RECESSED

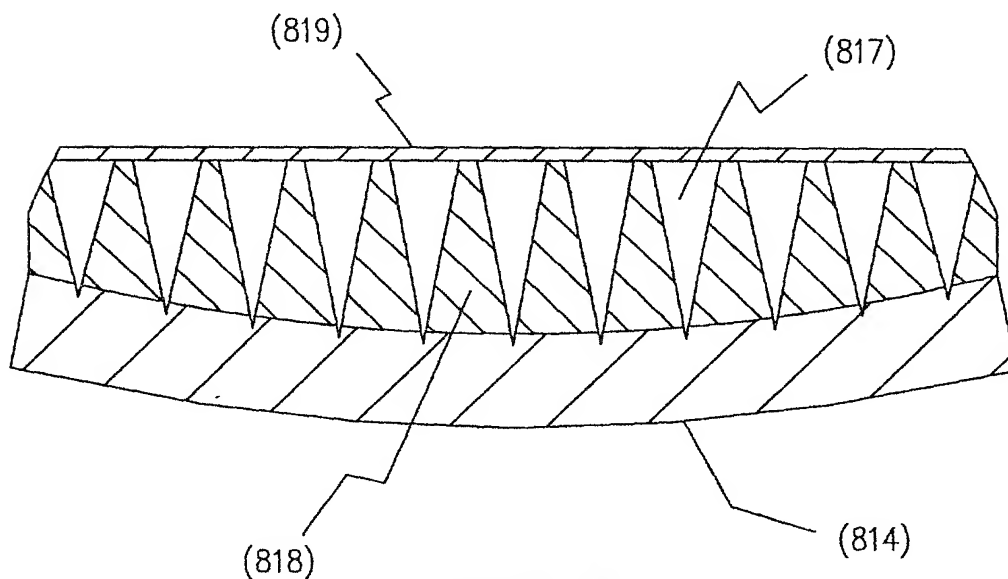

EPIRETINAL ELECTRODES - PENETRATING

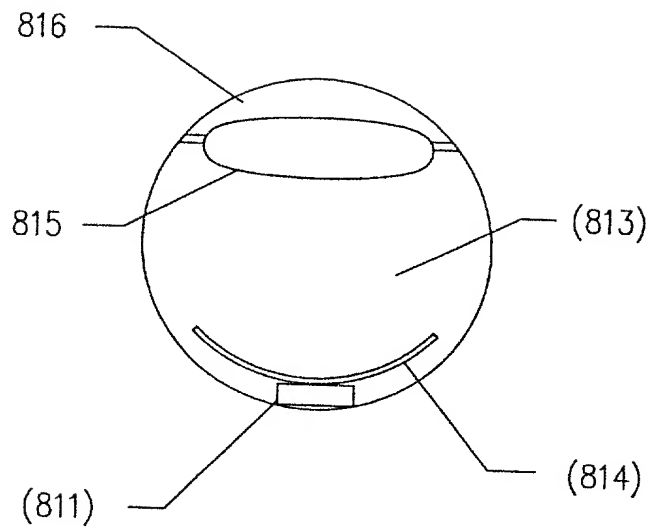


FIGURE 9a

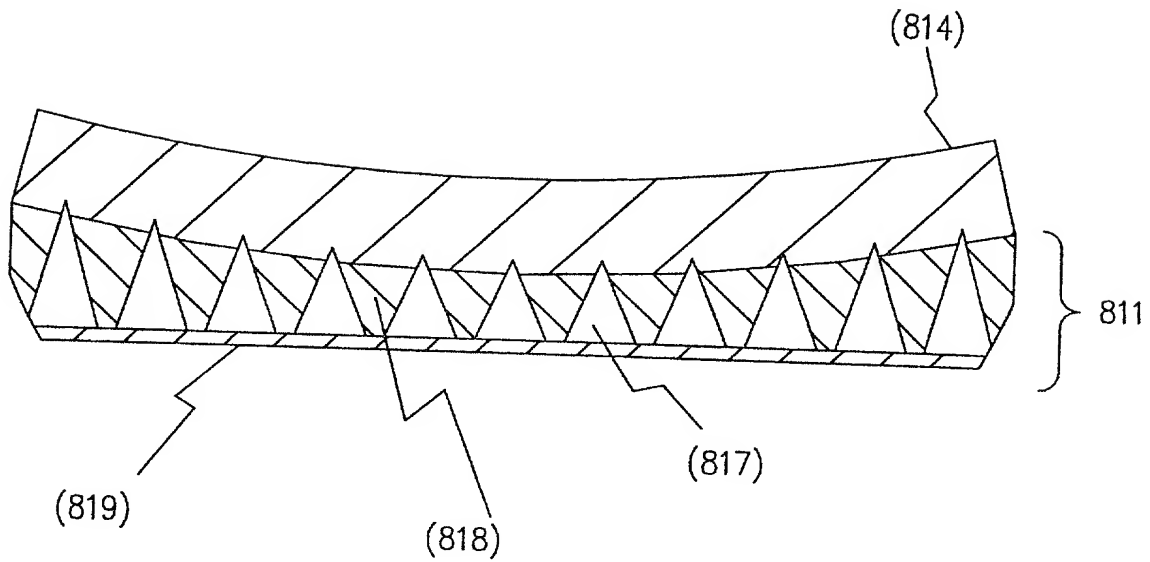


FIGURE 9b  
SUBRETINAL ELECTRODES — PENETRATING



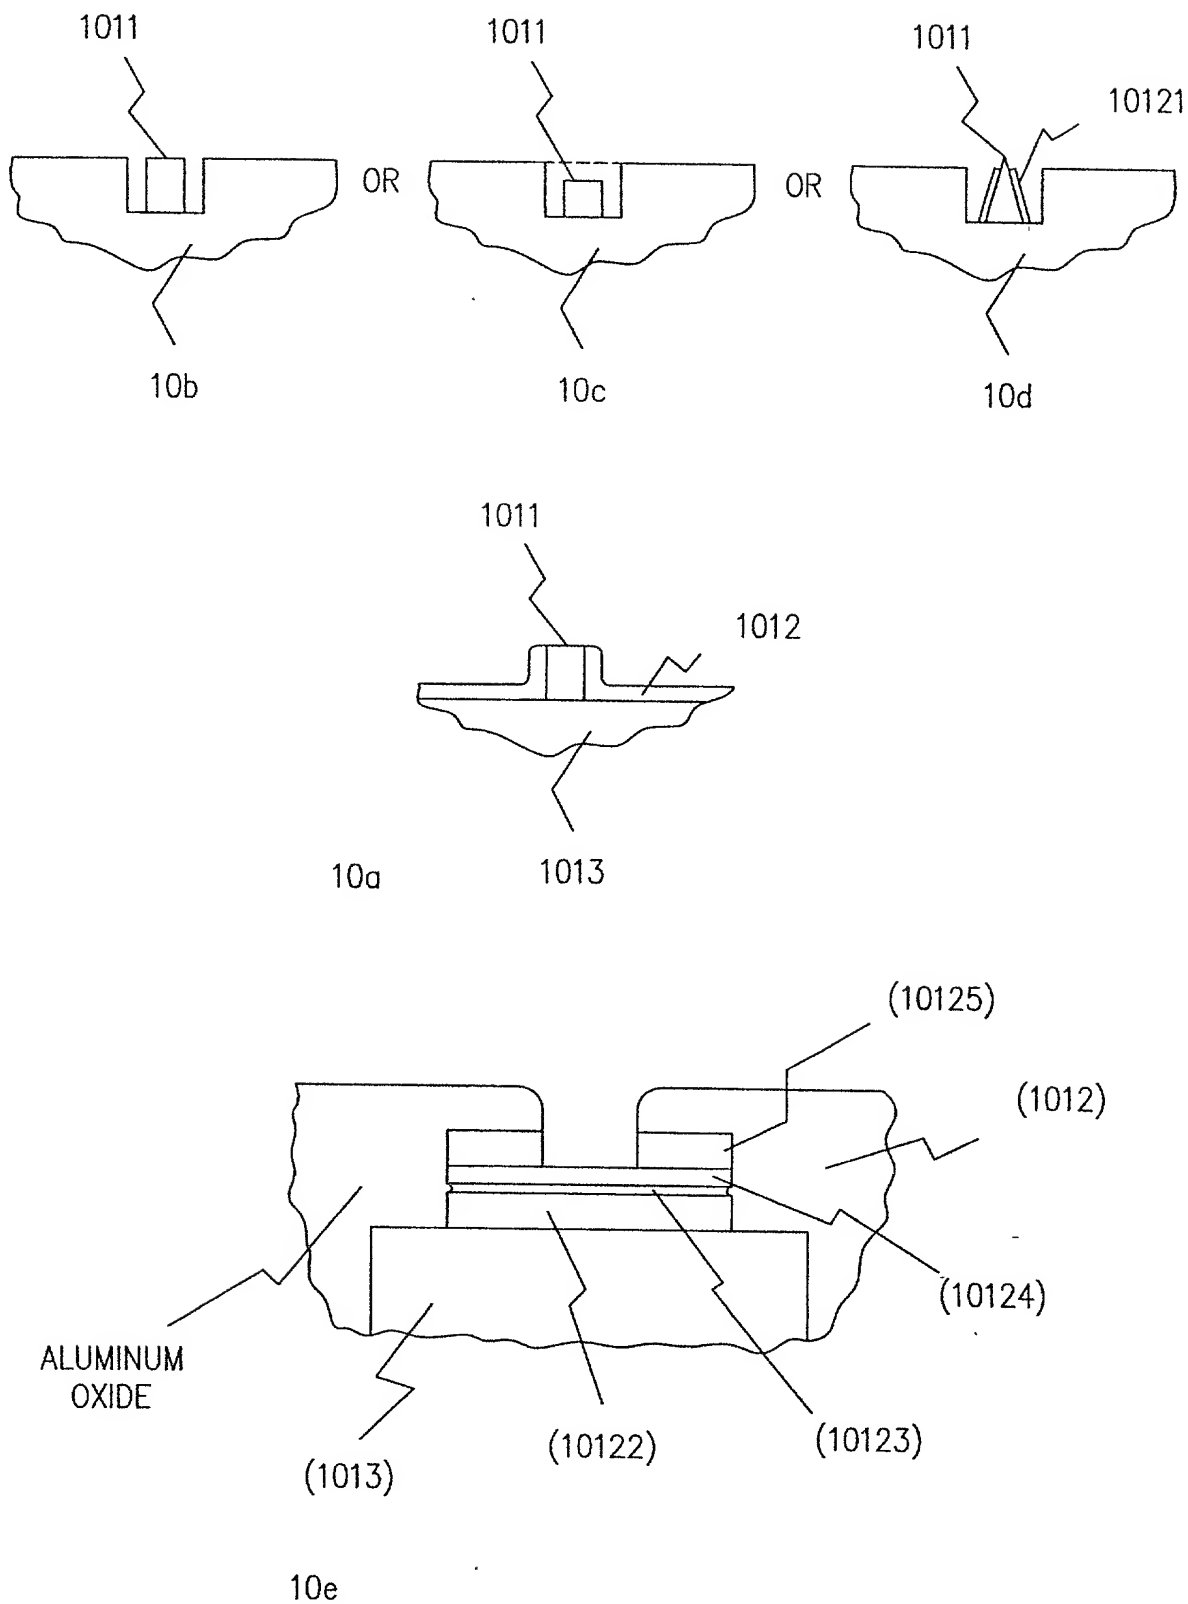


FIGURE 10

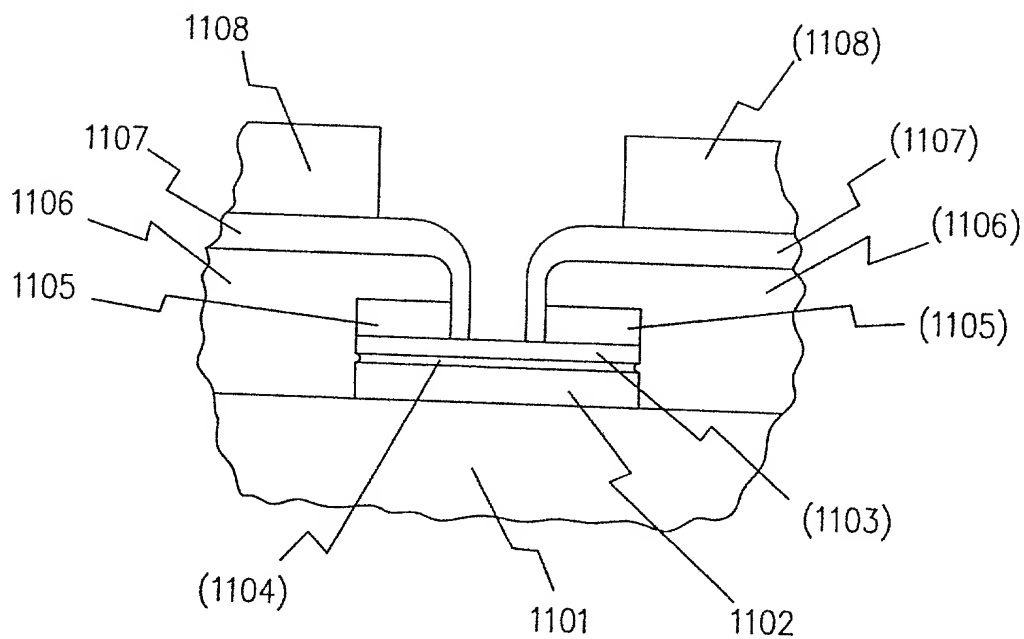


FIGURE 11a  
ELECTRODES

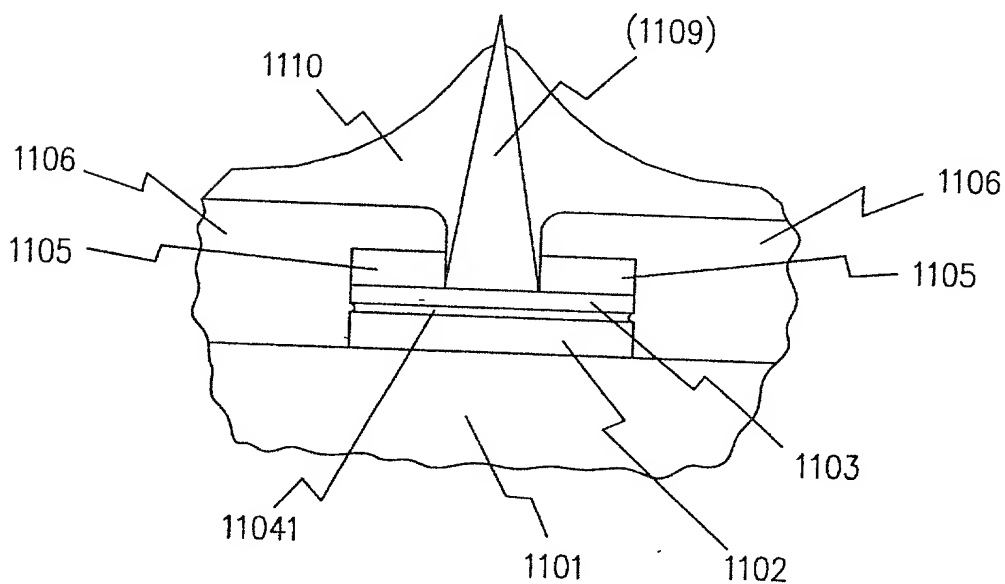


FIGURE 11b  
ELECTRODES

FIGURE 11

1033576-110901

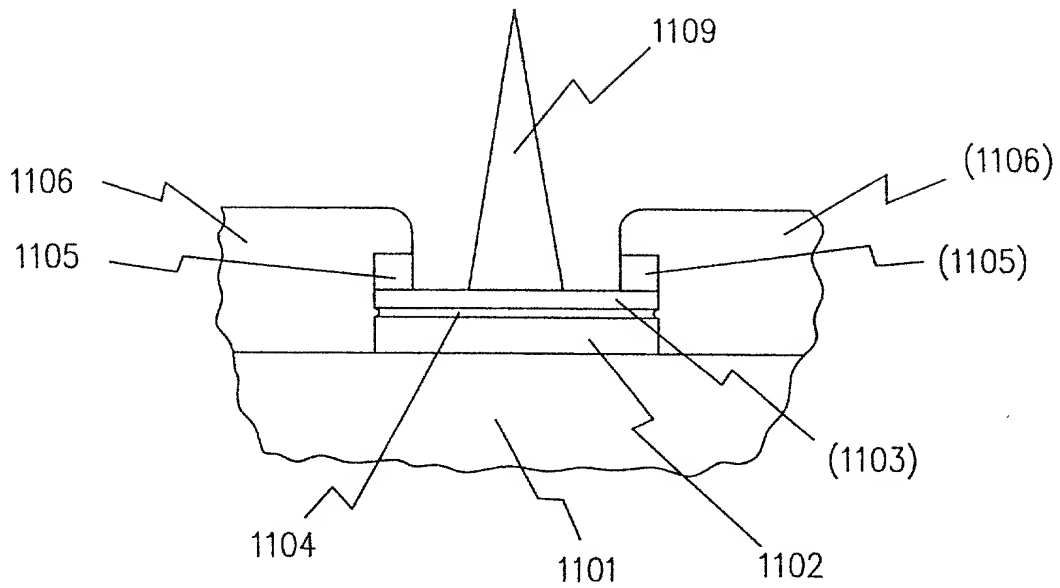


FIGURE 11c

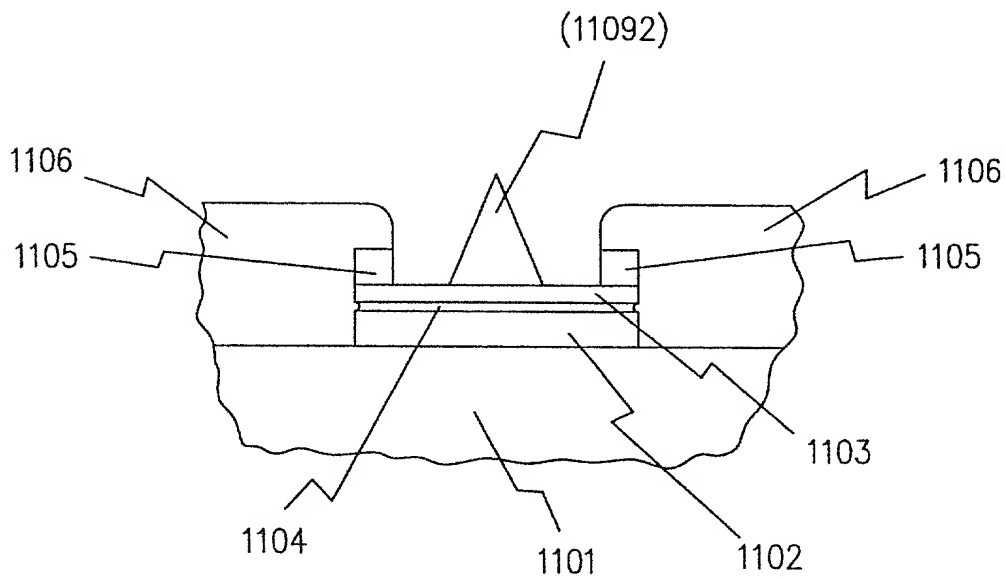


FIGURE 11d

FIG. 11e

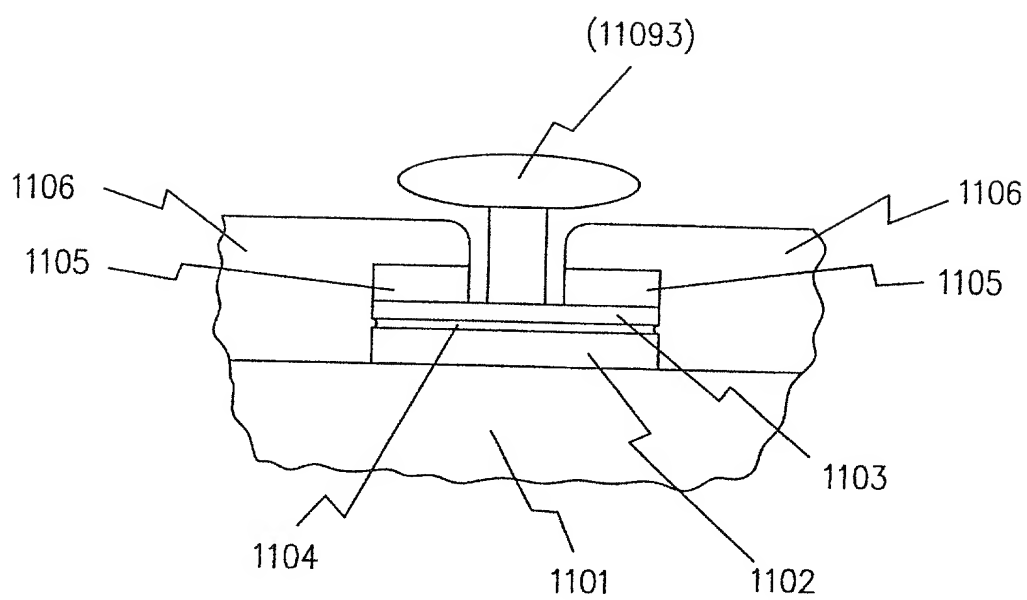


FIGURE 11e

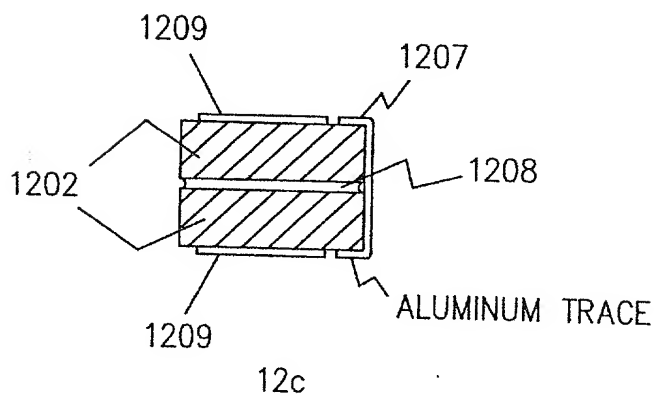
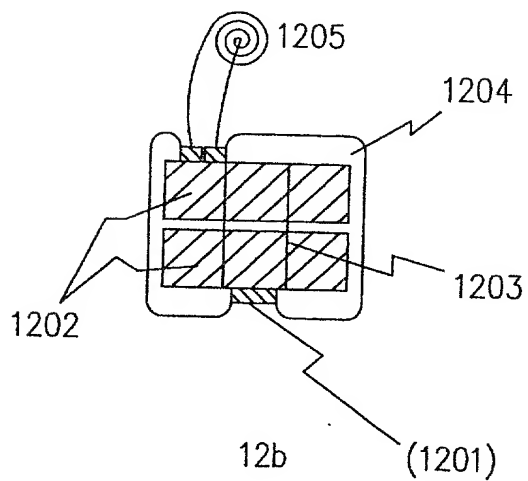
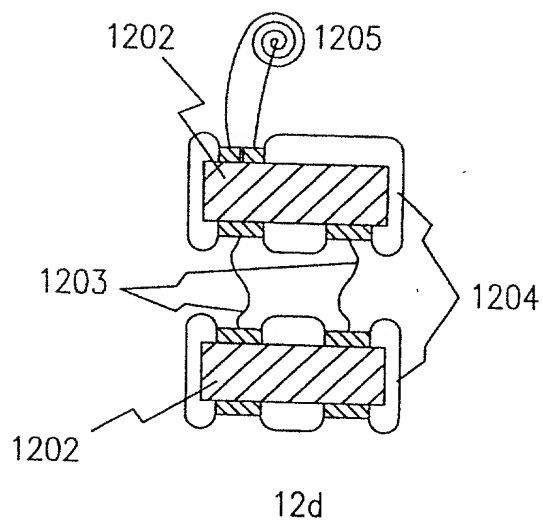
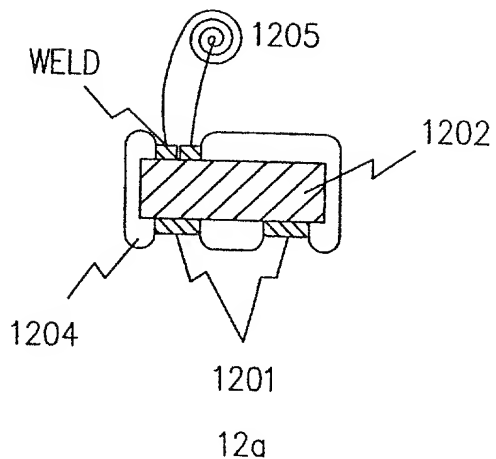


FIGURE 12  
COIL AND WIRE ATTACHMENT TO SUBSTRATES AT ELECTRODE

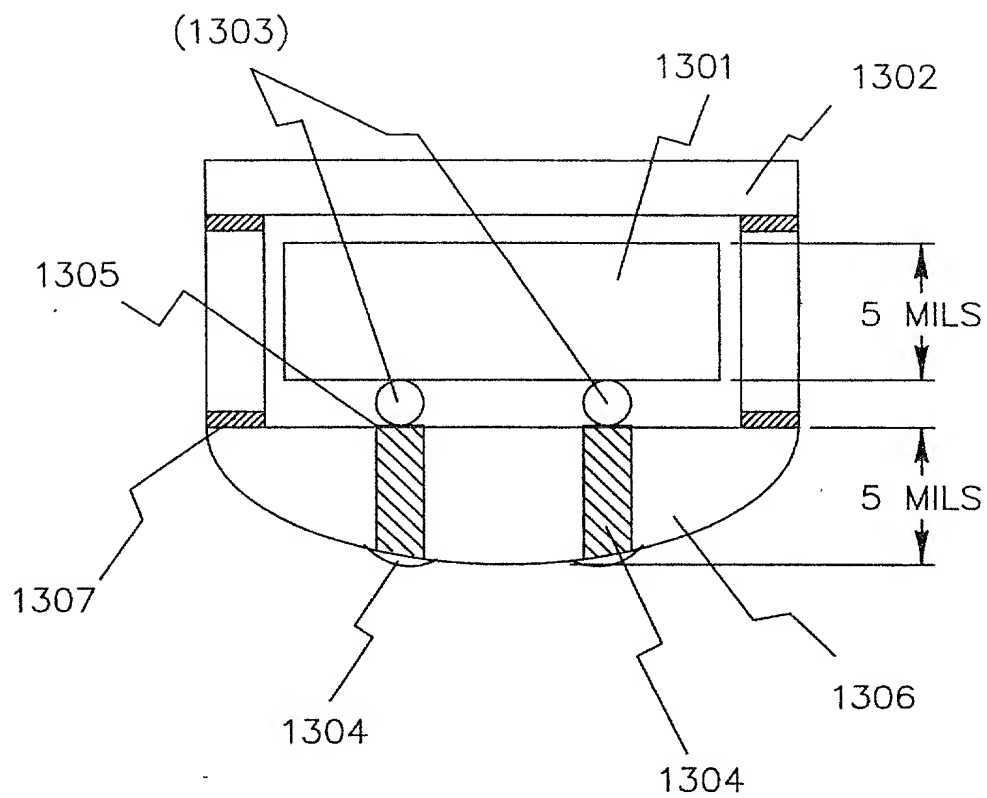


FIGURE 13  
HERMETIC SEALING

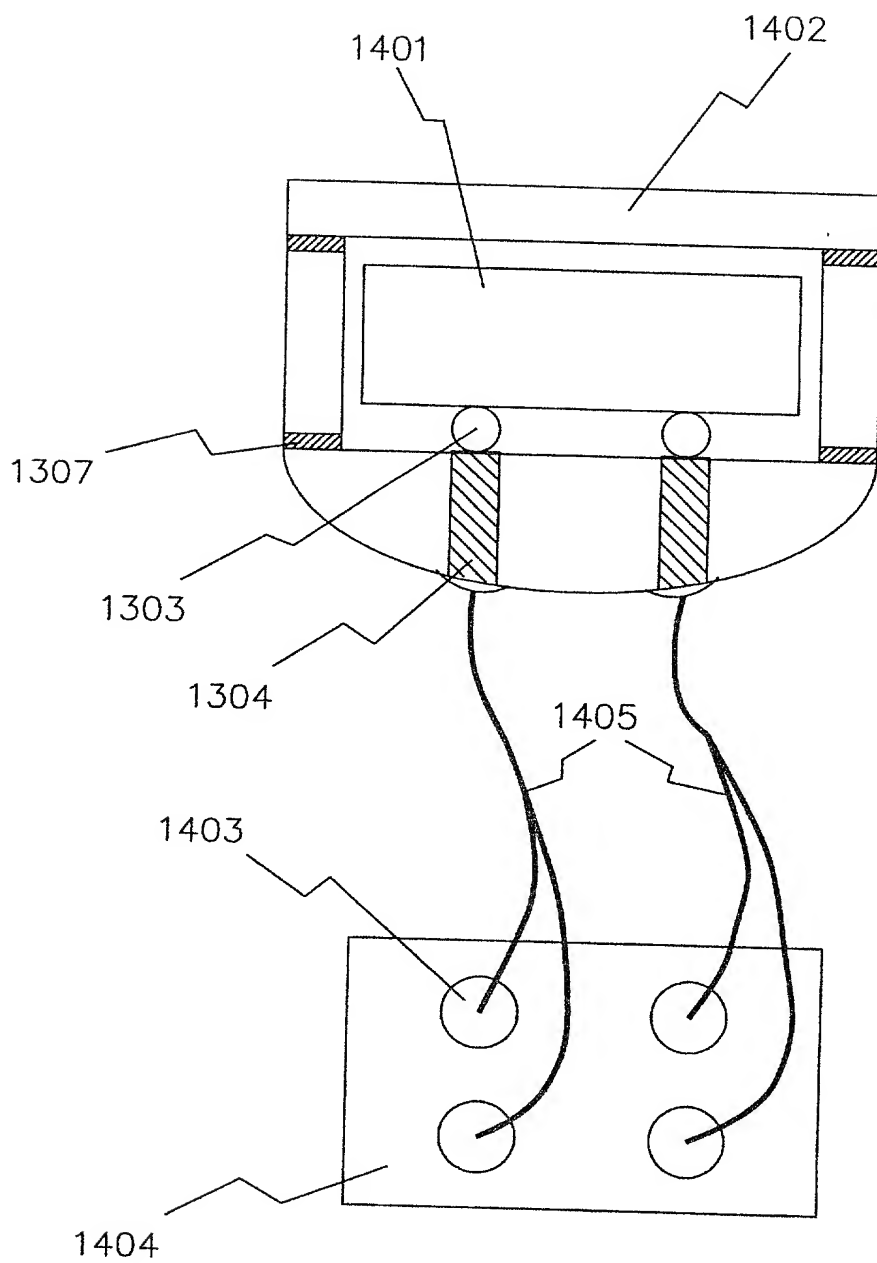


FIGURE 14

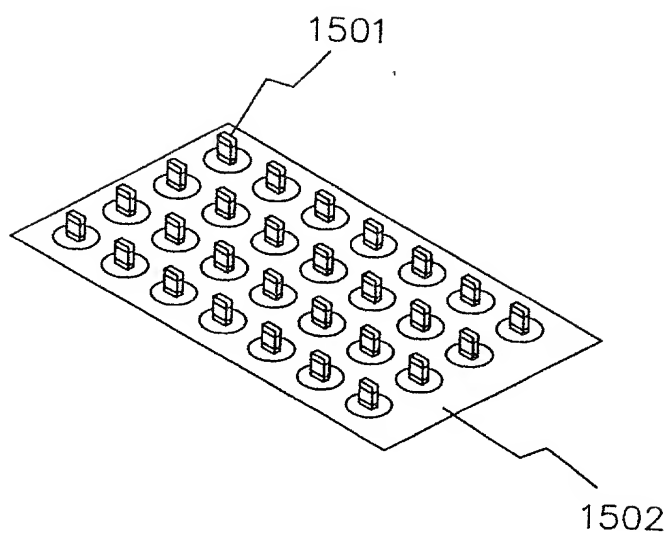


FIGURE 15



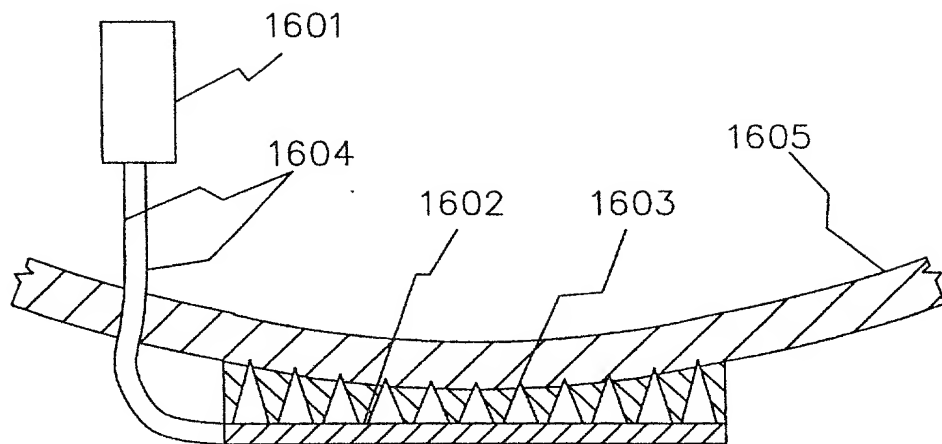


FIGURE 16a

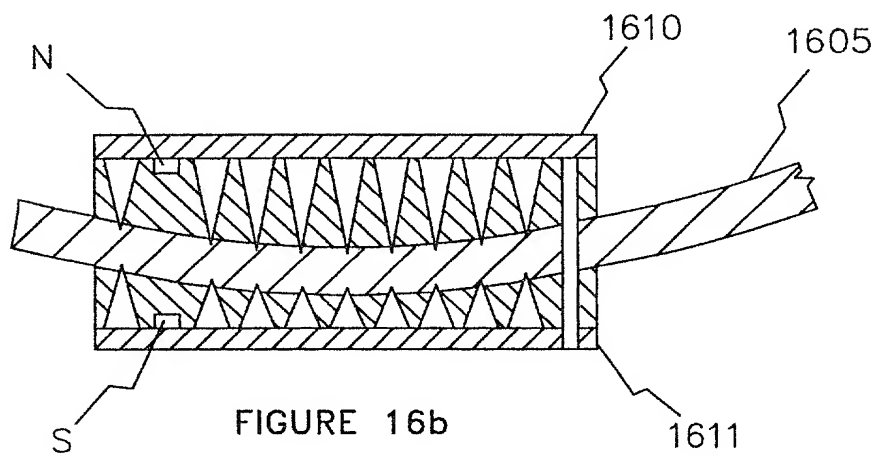


FIGURE 16b

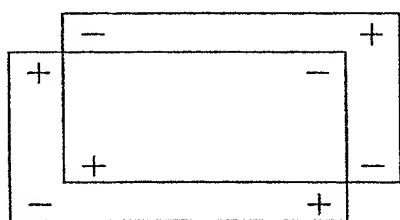


FIGURE 16c

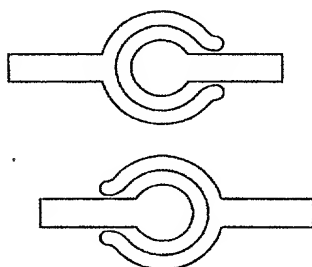


FIGURE 16d

PC PROGRAMMER

MAIN SCREEN


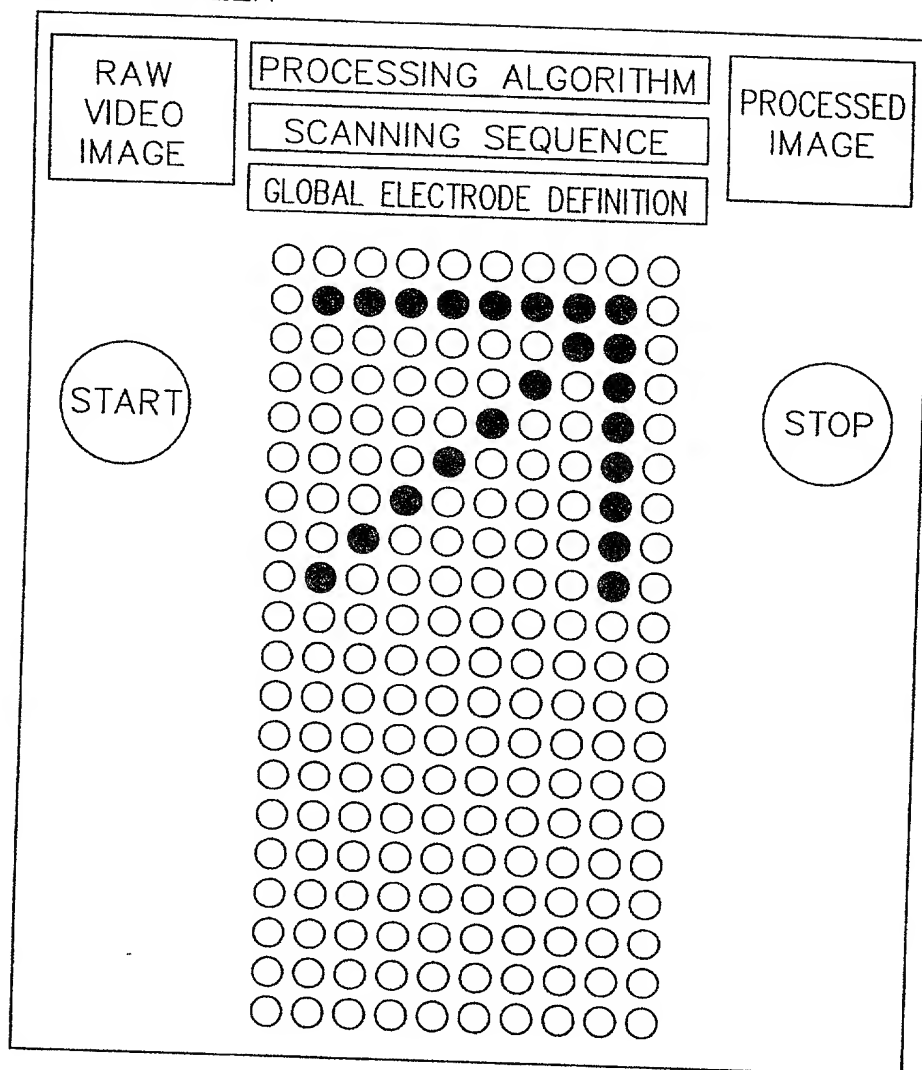


FIGURE 17a

# PROCESSING ALGORITHM

## PIXEL SELECTION

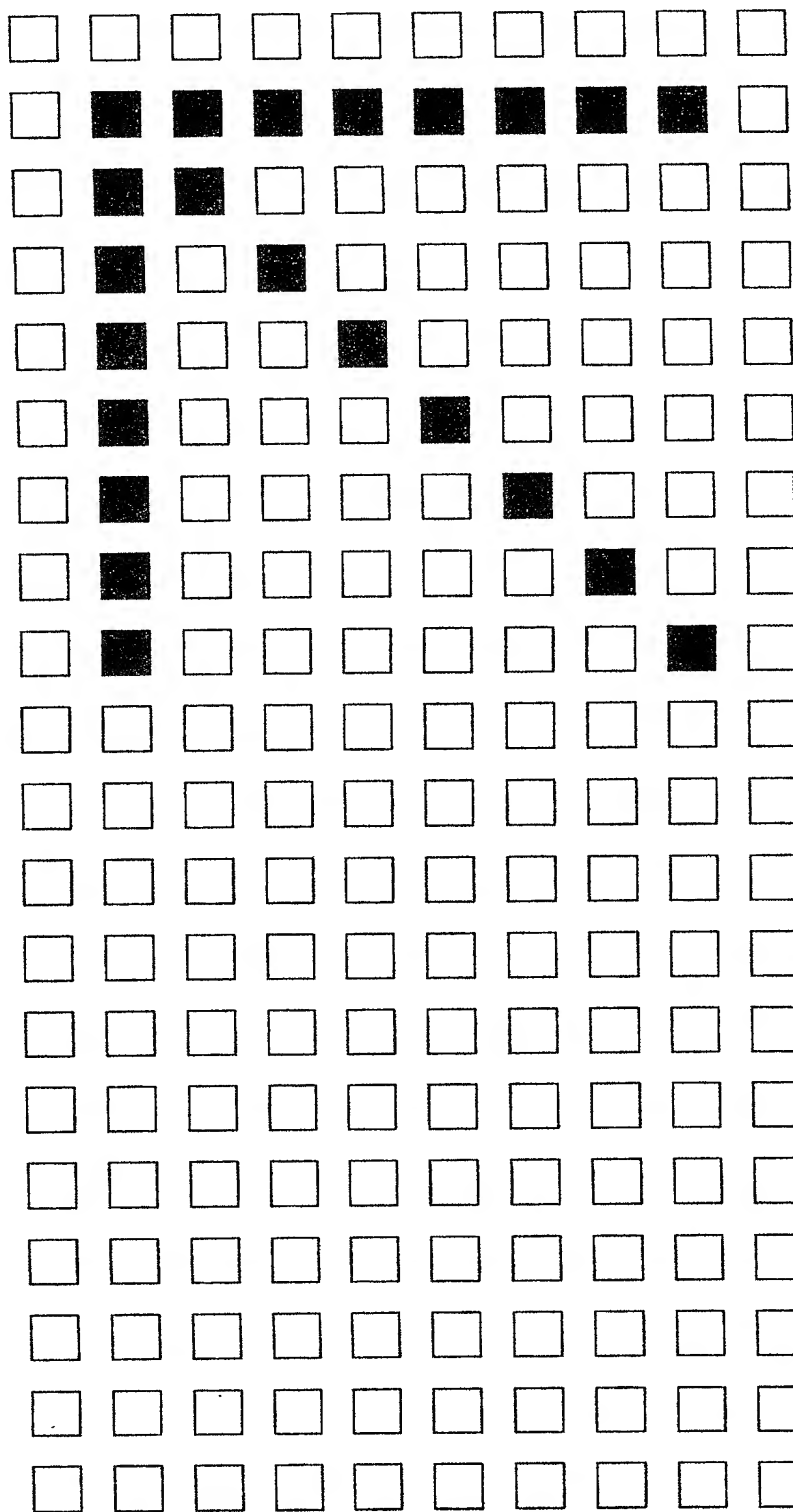


AVERAGE 8 SURROUNDING PIXELS

FIGURA 17b

10033576 110501

# SCANNING SEQUENCE

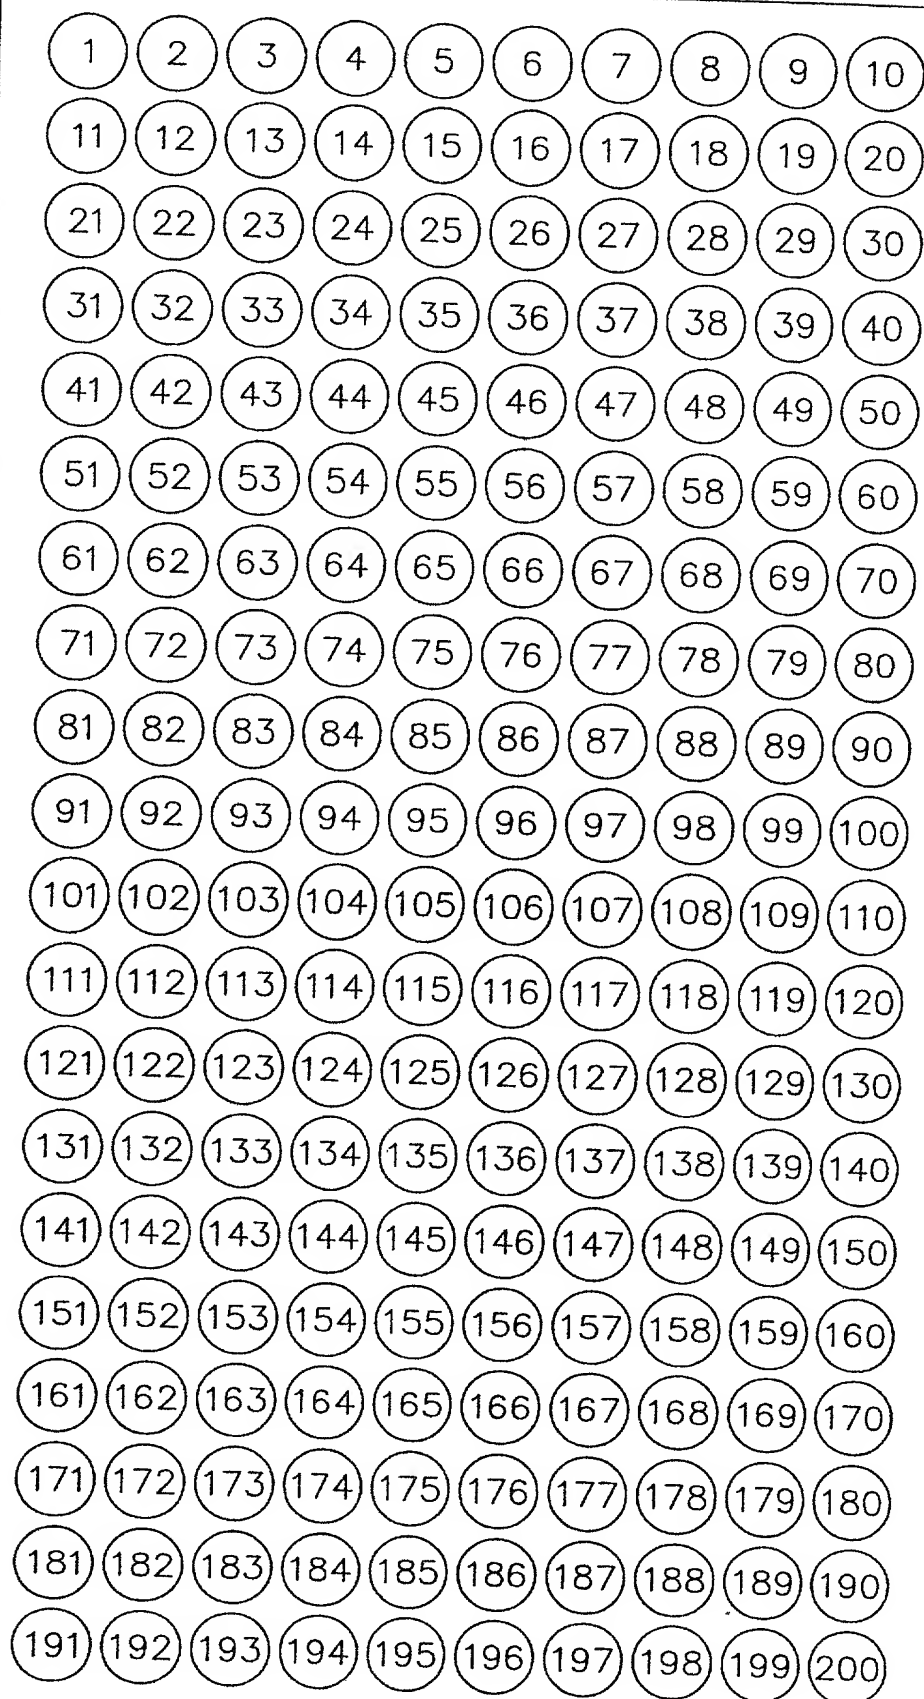

PREDEFINED SEQUENCE A

FIGURE 17c

# ELECTRODE PARAMETERS

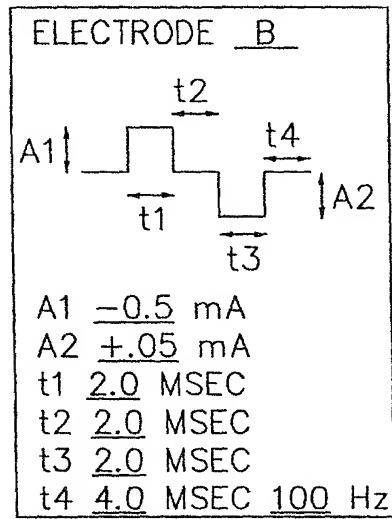


FIGURE 17d

# GLOBAL ELECTRODE CONFIGURATION

☐ MONOPOLAR  
☐ BIPOLAR  
☐ MULTIPOLAR

FIGURE 17e

## BIPOLAR

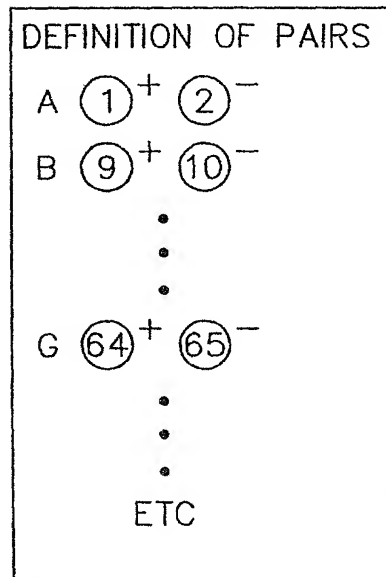


FIGURE 17f

## MULTIPOLAR

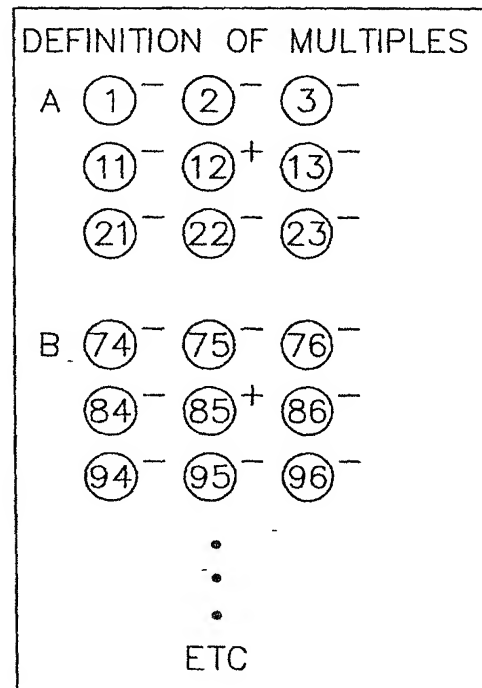


FIGURE 17g

40033576-410004

# PALM-SIZED TEST UNIT

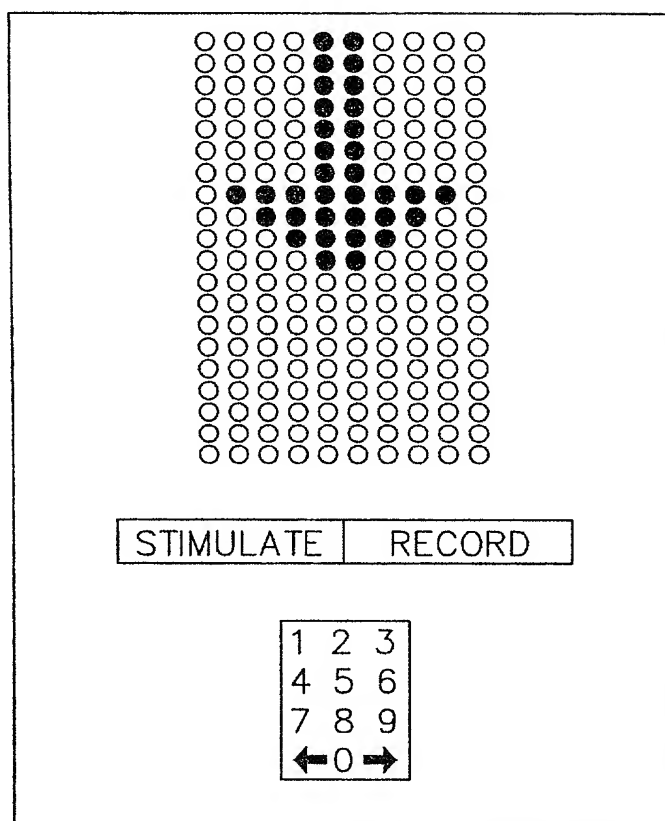


FIGURE 18a

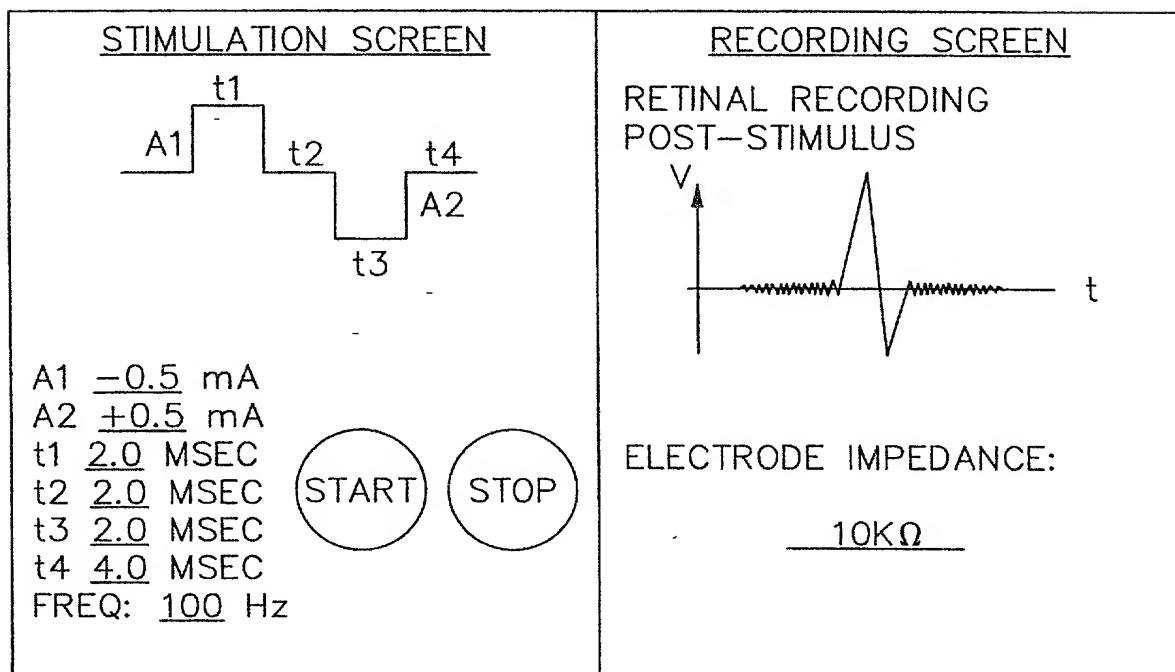


FIGURE 18b

FIGURE 18c

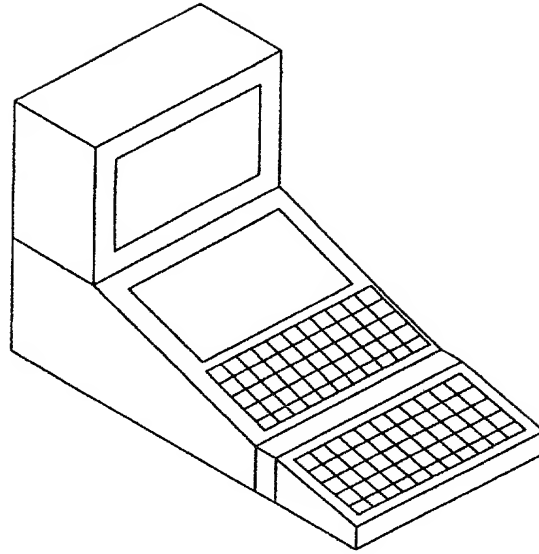


FIGURE 19a

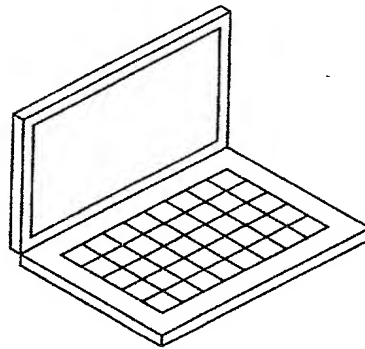


FIGURE 19b

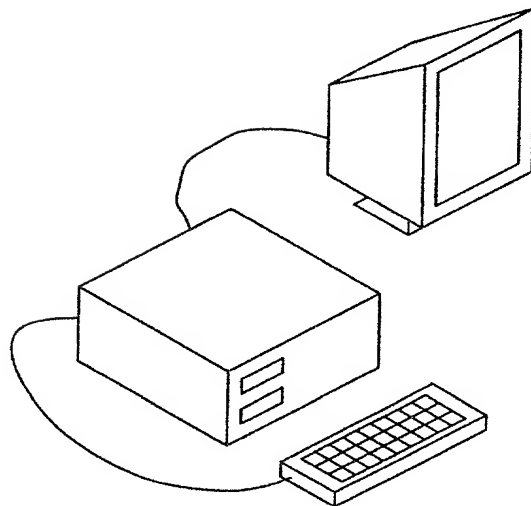


FIGURE 19c

PATIENT CONTROLLER

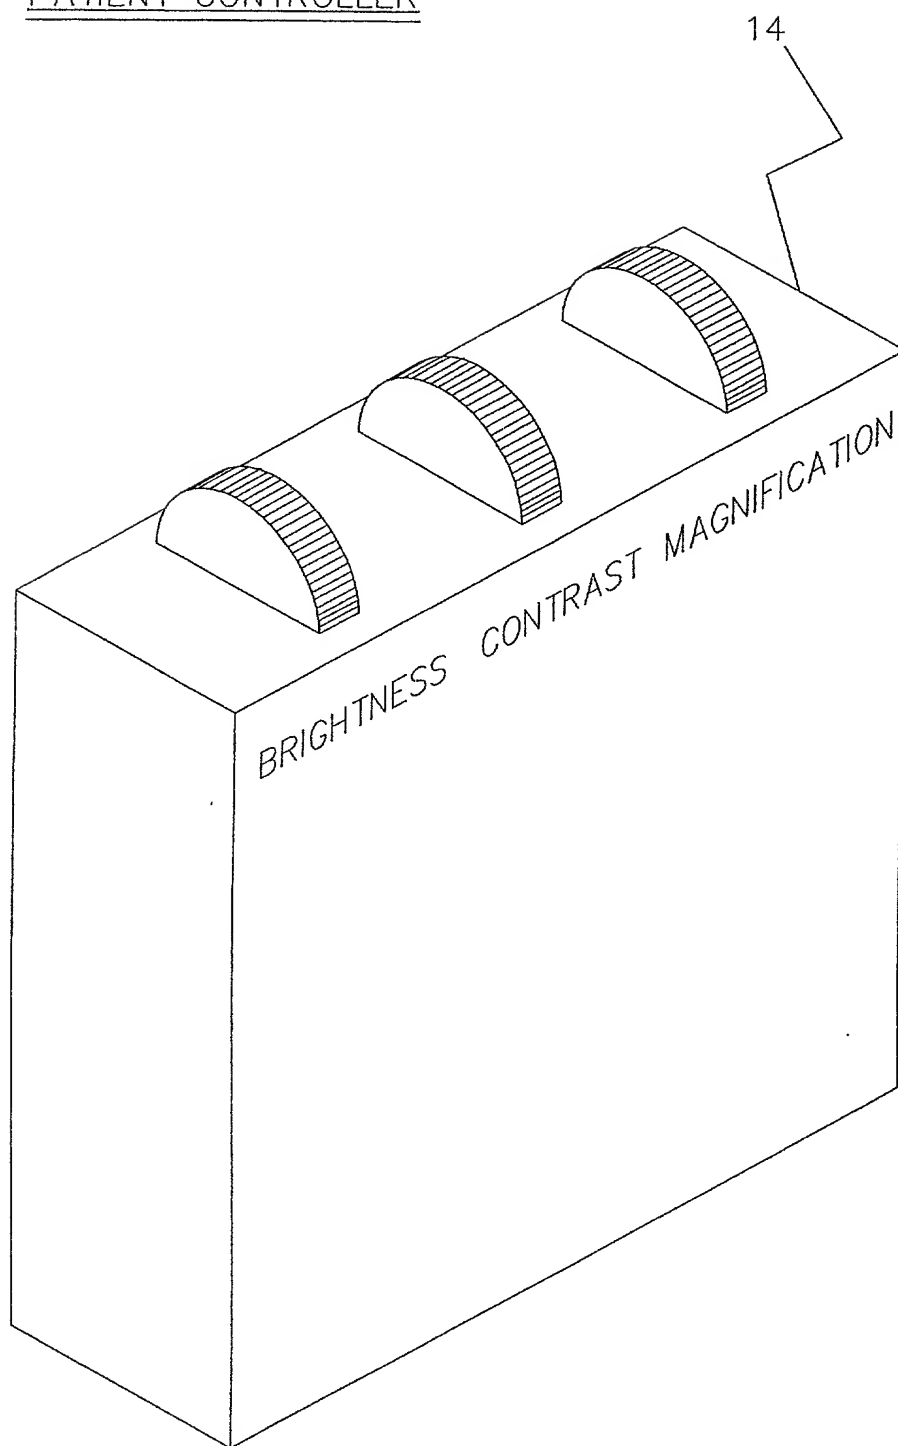


FIGURE 20